



Agilent 1260 Infinity High Performance Micro Autosampler

User Manual



Agilent Technologies

Notices

© Agilent Technologies, Inc. 2006, 2008, 2010, 2013

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

Manual Part Number

G1377-90001

Edition

11/2013

Printed in Germany

Agilent Technologies
Hewlett-Packard-Strasse 8
76337 Waldbronn

This product may be used as a component of an in vitro diagnostic system if the system is registered with the appropriate authorities and complies with the relevant regulations. Otherwise, it is intended only for general laboratory use.

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will

receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

In This Guide

This manual covers the Agilent 1260 Infinity High Performance Micro Autosampler (G1377A).

1 Introduction

This chapter gives an introduction to the High Performance Micro Autosampler.

2 Site Requirements and Specifications

This chapter describes the site requirements and specifications of the High Performance Micro Autosampler.

3 Installing the Autosampler

This chapter describes the installation of the High Performance Micro Autosampler.

4 Using the Autosampler

This chapter describes the usage of the High Performance Micro Autosampler.

5 Optimizing Performance

This chapter provides information on how to optimize the autosampler.

6 Troubleshooting and Diagnostics

This chapter gives an overview to troubleshooting the High Performance Micro Autosampler.

7 Error Information

This chapter describes the meaning of error messages, and provides information on probable causes and suggested actions how to recover from error conditions.

In This Guide

8 Maintenance

This chapter describes the maintenance of the autosampler.

9 Parts for Maintenance

This chapter provides information on parts for maintenance.

10 Identifying Cables

This chapter provides information on cables used with the Agilent 1200 Infinity Series modules.

11 Hardware Information

This chapter describes the module in more detail on hardware and electronics.

12 Appendix

This appendix provides general safety and environmental information.

Contents

1	Introduction	9
	Introduction to the Autosampler	10
	Sampling Sequence	12
	Sampling Unit	16
	Needle/Sample Transport Assembly	20
	Advanced Operating Modes	22
	System Overview	24
2	Site Requirements and Specifications	27
	Site Requirements	28
	Physical Specifications	31
	Performance Specifications	32
3	Installing the Autosampler	33
	Unpacking the Sampler	34
	Optimizing the Stack Configuration	36
	Installation Information on Leak and Waste Handling	41
	Installing the Autosampler	45
	Installing a Thermostatted Autosampler	48
	Flow Connections to the Sampler	52
	Installing the Sample Tray	54
	Transporting the Sampler	56
4	Using the Autosampler	57
	Leak and Waste Handling	58
	Sample Trays	59
	List of Recommended Plates and Closing Mat	60
	List of Recommended Vials and Caps	62
	Configure Well Plate Types	64
	Turn ON and Initialization Steps	67

5	Optimizing Performance	69
	Optimizing Performance	70
	Optimization for Lowest Carry-Over	71
	Fast Injection Cycle and Low Delay Volume	78
	Precise Injection Volume	80
	Choice of Rotor Seal	82
	Choice of Seat Capillary	83
6	Troubleshooting and Diagnostics	85
	Overview of the Sampler's Indicators and Test Functions	86
	Status Indicators	88
	Maintenance Functions	90
	Step Commands	92
	Troubleshooting the Autosampler	94
	Errors Which May Occur During the Turn ON and Initialization Process	95
	Instrument Logbook Errors and Step by Step Repair Proces	99
	Needle Centering Over the Vial or the Well	104
	Agilent Lab Advisor Software	105
7	Error Information	107
	What Are Error Messages	109
	General Error Messages	110
	Module Specific Error Messages	116
8	Maintenance	129
	Introduction to Maintenance	130
	Warnings and Cautions	131
	Cleaning the Module	133
	Maintenance Functions	134
	Maintenance Procedures	135
	Removing the Needle Assembly	136
	Installing the Needle Assembly	138
	Removing the Needle Carrier Assembly	140
	Installing the Needle Carrier Assembly	141
	Exchanging the Needle Seat	142
	Exchanging the Seat Capillary	144
	Exchanging the Rotor Seal	145

Metering Seal and Plunger	146
Removing the Loop Capillary	148
Installing the Loop Capillary	150
Replacing the Peristaltic Pump	152
Installing Interface Board	153
Replacing Module Firmware	154
9 Parts for Maintenance	155
Sampler Main Assemblies	156
Vial Trays	158
Accessory Kits	160
Thermostat for ALS/FC/Spotter	161
10 Identifying Cables	163
Cable Overview	164
Analog Cables	166
Remote Cables	168
BCD Cables	171
CAN/LAN Cables	173
External Contact Cable	174
RS-232 Cables	175
Agilent 1200 Module to Printer	176
11 Hardware Information	177
Firmware Description	178
Electrical Connections	181
Interfaces	183
Setting the 8-bit Configuration Switch (without On-board) LAN	190
Optional Interface Boards	194
Instrument Layout	198
Early Maintenance Feedback	199

12 Appendix 201

General Safety Information	202
The Waste Electrical and Electronic Equipment Directive	205
Lithium Batteries Information	206
Radio Interference	207
Sound Emission	208
Use of Solvents	209
Agilent Technologies on Internet	210



1 Introduction

Introduction to the Autosampler	10
Sampling Sequence	12
Injection Sequence	14
Sampling Unit	16
Analytical Head	17
Injection-Valve	18
Needle Flush Station	19
Needle Lock	19
Needle/Sample Transport Assembly	20
Advanced Operating Modes	22
System Overview	24
Leak and Waste Handling	24

This chapter gives an introduction to the High Performance Micro Autosampler.



Introduction to the Autosampler

The Agilent 1260 Infinity High Performance Micro Autosampler is designed to perform capillary LC with injection of sample volumes ranging from nL to μ L.

Features: A micro Rheodyne® valve and the optimized design of the needle seat, loop and seat capillaries minimize dispersion. A high-resolution metering device offers resolution ten times better than a standard autosampler, bypass operation facilitates low delay volume, increased sample injection speed for high sample throughput, flexible and convenient sample handling with different types of sample containers. Using 384-well plates allows to process up to 768 samples unattended.

Technical Principle: The well plate sampler transport mechanism uses an X-Z-theta robot to optimize the positioning of the sampling arm on the well plate. Once the sampling arm is positioned over the programmed sample position, the programmed sample volume is drawn by the metering device into the sampling needle. The sampling arm then moves to the injection position where the sample is flushed onto the column.

The autosamplers employ a vial/plate pusher mechanism to hold down the vial or the plate while the needle is drawn back from the sample vessel (a must in the case a septum is used). This vial/plate pusher employs a sensor to detect the presence of a plate and to ensure accurate movement regardless of plate used. All axes of the transport mechanism (x-,z-,theta-robot) are driven by stepper-motors. Optical encoders ensure the correct operation of the movement.

The micro metering device provides injection volumes from 0.01 – 8 μ L with the standard loop capillary installed and from 0.01 – 40 μ L with the extended loop capillary. The entire flowpath including the metering device is always flushed by the mobile phase after injection for minimum internal carry-over.

An additional needle flush station with a peristaltic pump is installed to wash the outside of the needle. This reduces the already low carry-over for very sensitive analysis. The bottle containing the mobile phase for the wash procedure will be located in the solvent bottle cabinet. Produced waste during this operation is channeled safely away through a waste drain.

The six-port (only 5 ports are used) injection valve unit is driven by a high-speed hybrid stepper motor. During the sampling sequence, the valve unit bypasses the autosampler, and connects flow from the pump to the column directly. During injection and analysis, the valve unit directs the flow through the autosampler which ensures that all of the sample is injected onto the column, and that the metering unit and needle are always free from sample residue before the next sampling sequence begins. All the injection valves have different stator heads and different rotor seals. The volume of each valve is different.

Control of the vial/plate temperature in the thermostatted autosampler is achieved using an additional Agilent module; the Agilent 1290 Infinity Thermostat for ALS/FC/Spotter.

The thermostat contains Peltier-controlled heat-exchangers. A fan draws air from the area above the sample vial tray of the autosampler. It is then blown through the fins of the cooling/heating module. There it is cooled or heated according the temperature setting. The thermostatted air enters the autosampler through a recess underneath the special designed sample tray. The air is then distributed evenly through the sample tray ensuring effective temperature control, regardless of how many vials are in the tray. In cooling mode condensation is generated on the cooled side of the Peltier elements. This condensed water is safely guided into a waste bottle for condensed water.

Sampling Sequence

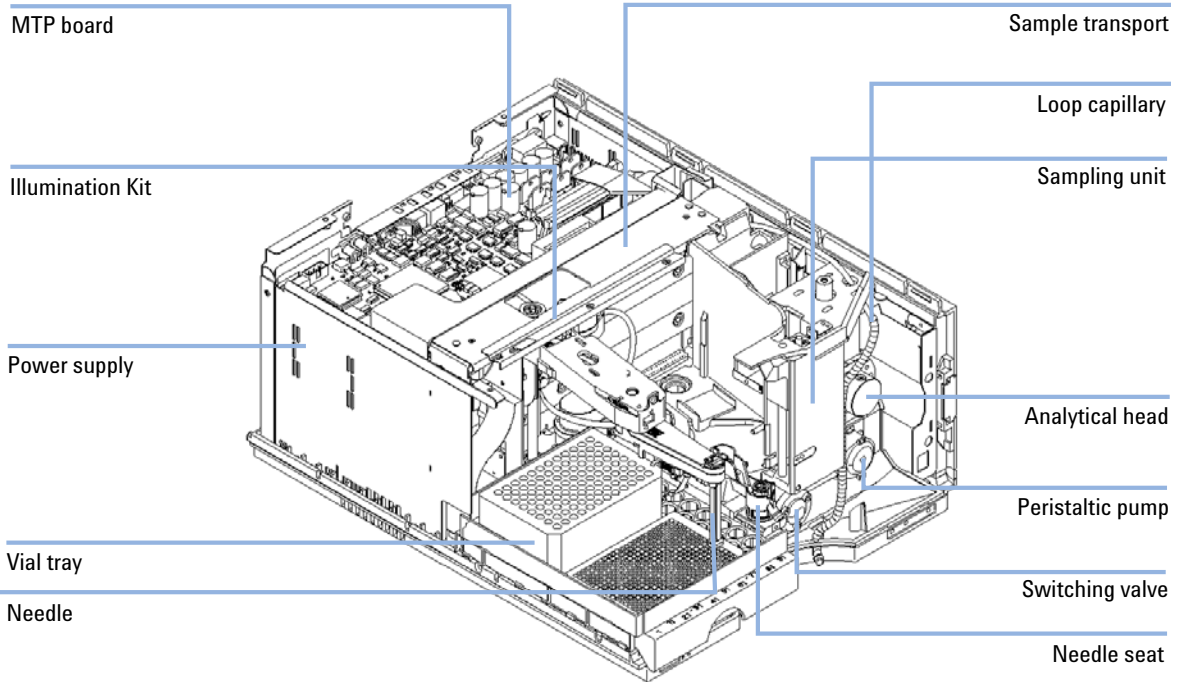


Figure 1 Overview of the autosampler

The movements of the autosampler components during the sampling sequence are monitored continuously by the autosampler processor. The processor defines specific time windows and mechanical ranges for each movement. If a specific step of the sampling sequence is not completed successfully, an error message is generated. Solvent is bypassed from the autosampler by the injection valve during the sampling sequence. The needle moves to the desired sample vial position and is lowered into the sample liquid in the vial to allow the metering device to draw up the desired volume by moving its plunger back a certain distance. The needle is then raised again and moved onto the seat to close the sample loop. Sample is applied to the column when the injection valve returns to the mainpass position at the end of the sampling sequence.

The standard sampling sequence occurs in the following order:

- 1** The injection valve switches to the bypass position.
- 2** The plunger of the metering device moves to the initialization position.
- 3** The needle lock moves up.
- 4** The needle moves to the desired sample vial position.
- 5** The needle lowers into the vial.
- 6** The metering device draws the preset sample volume.
- 7** The needle lifts out of the vial.
- 8** The needle is then moved onto the seat to close the sample loop.
- 9** The needle lock moves down.
- 10** The injection cycle is completed when the injection valve switches to the mainpass position.

If needle wash is required it will be done between step 7 and 8.

Injection Sequence

Before the start of the injection sequence, and during an analysis, the injection valve is in the mainpass position (Figure 2 on page 14). In this position, the mobile phase flows through the autosampler metering device, sample loop, and needle, ensuring all parts in contact with sample are flushed during the run, thus minimizing carry-over

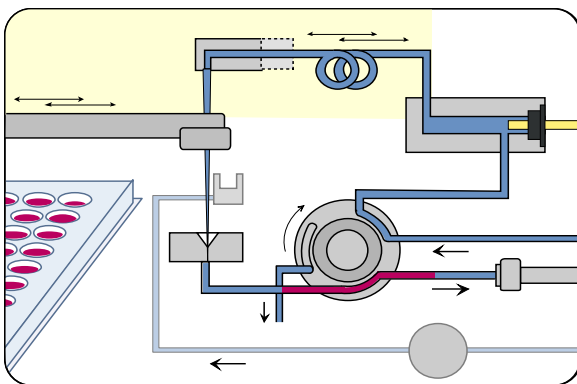


Figure 2 Mainpass Position

When the sample sequence begins, the valve unit switches to the bypass position (Figure 3 on page 14). Solvent from the pump enters the valve unit at port 1, and flows directly to the column through port 6.

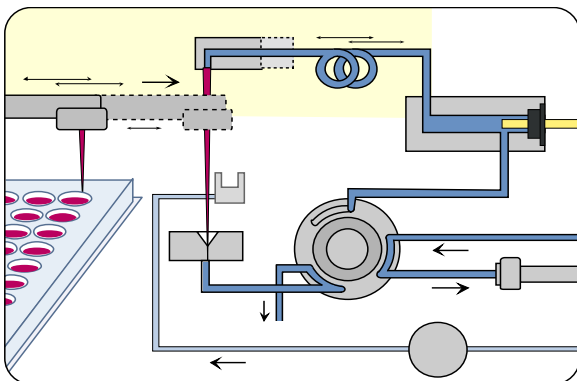


Figure 3 Bypass Position

The standard injection starts with „draw sample from vial”. In order to do this the needle moves to the desired sample vial position and is lowered into the sample liquid in the vial to allow the metering device to draw up the desired volume by moving its plunger back a certain distance. The needle is then raised again and moved onto the seat to close the sample loop. In case of an injector program several steps are interspersed at this point.

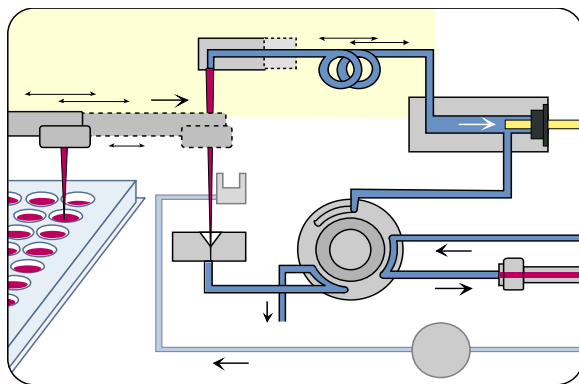


Figure 4 Drawing the Sample

Flush the Needle

Before injection and to reduce the carry-over for very sensitive analysis, the outside of the needle can be washed in a flush port located behind the injector port on the sampling unit. As soon the needle is on the flush port a peristaltic pump delivers some solvent during a defined time to clean the outside of the needle. At the end of this process the needle returns to the injection port.

Inject-and-Run

The final step is the inject-and-run step. The six-port valve is switched to the main-pass position, and directs the flow back through the sample loop, which now contains a certain amount of sample. The solvent flow transports the sample onto the column, and separation begins. This is the beginning of a „run” within an analysis. In this stage, all major performance-influencing hardware is flushed internally by the solvent flow. For standard applications no additional flushing procedure is required.

Sampling Unit

The sampling unit consists of subsystems as well. The main carrier part is a die casting part which carries the following functional elements.

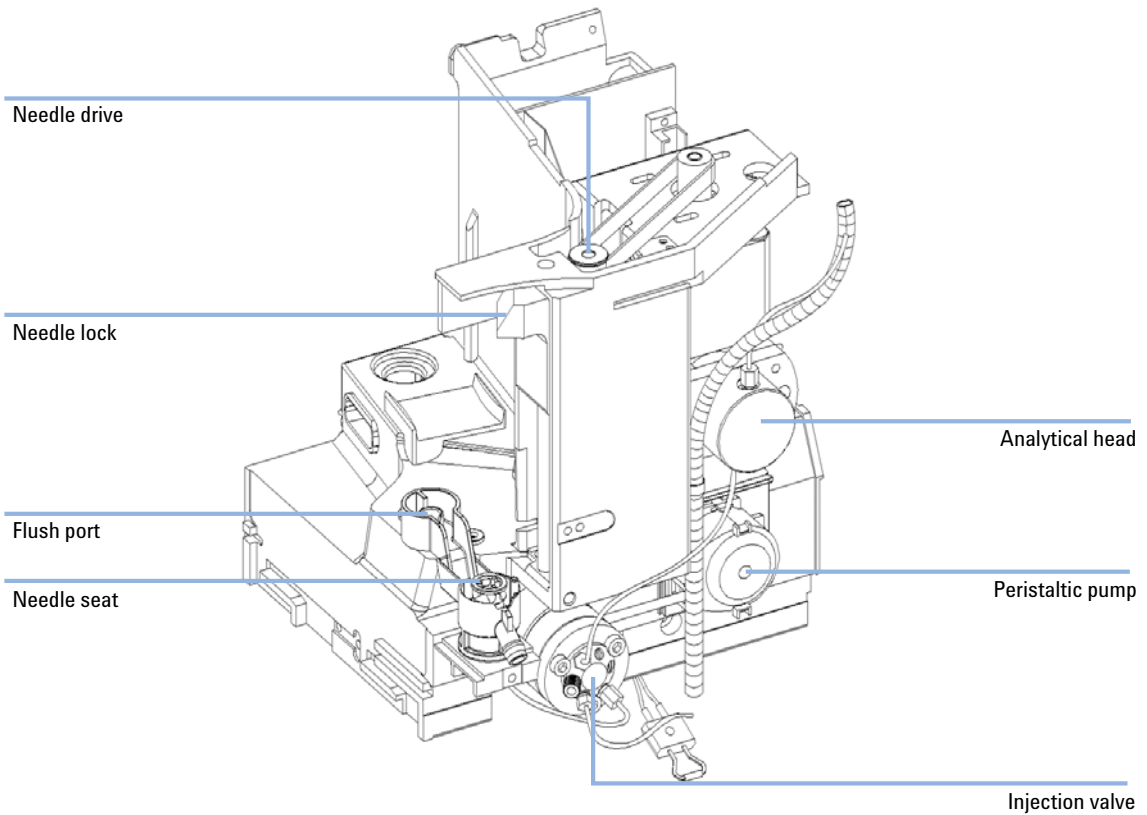


Figure 5 Sampling unit

Analytical Head

The analytical head is driven by the stepper motor that is connected to the drive shaft by a toothed belt. The drive nut on the spindle converts the circular movement of the spindle to linear motion. The drive nut pushes the sapphire plunger against the tension of the spring into the analytical head. The base of the plunger sits on the large bearing of the drive nut, which ensures the plunger is always centered. A ceramic ring guides the movement of the plunger in the analytical head. The home position of the plunger is sensed by an infra-red sensor on the sampling unit flex board while the sample volume is determined by counting the number of steps from the home position (7 nL/motor step). The backward movement of the plunger (driven by the spring) draws sample from the vial.

To reduce potential user mistakes, different versions of analytical heads are recognized by RF-tags sitting on the exchangeable assembly. The G1377A High Performance Micro Autosampler must only be used with the Micro Analytical Head (Analytical Head Assembly (40 µL) (G1377-60013)).

Table 1 Analytical head Technical Data

	Standard 100 µl (G1367-60003)	High Pressure 40µl (G1377-60023)	Micro 40 µl (G1377-60013)
Number of steps	15000	15000	60000
Volume resolution	14 nl/motor step	5.6 nl/motor step	1.4 nl/motor step
Maximum stroke	100 µl	40 µl	40 µl
Pressure limit	400 bars	600 bars	400 bars
Plunger material	Sapphire	Sapphire	Sapphire

Injection-Valve

A high pressure 6-port/2-position-valve to direct streams of mobile phase and sample to different directions (e.g. via loop to column or directly to column).

The two-position 6-port injection valve is driven by a stepper motor. Only five of the six ports are used (port 3 is not used). A lever/slider mechanism transfers the movement of the stepper motor to the injection valve. Two microswitches monitor switching of the valve (bypass and mainpass end positions). The injection valve has a ceramic stator, Vespel rotor seal (Tefzel seal available), and stainless-steel head. Three screws hold the head and internal components in place. No valve adjustments are required after replacing internal components.

Table 2 Injection-Valve Technical Data

	Standard (0101-0921)	Micro (0101-1050)	High pressure (0101-1422)
Motor type	4 V, 1.2 A stepper motor	4 V, 1.2 A stepper motor	4 V, 1.2 A stepper motor
Seal material	Vespel™ or Tefzel™	Vespel™	PEEK
Stator material	Ceramic/PEEK	Head coated SST	Ultralife
Number of ports	6	6	6
Switching time	< 150 ms	< 150 ms	< 150 ms

Needle Flush Station

A needle flush station to wash the outer surface of the injection needle and a peristaltic pump to deliver fresh solvent to the wash station. (The reservoir for the solvent is located in the solvent cabinet, the waste is channeled by a separate flex tube to a waste bottle.

Needle Lock

A needle lock is used to support the needle carrier in its function making a firm seal of the needle in its seat.

The needle lock arm is driven by a stepper motor connected to the spindle assembly by a toothed belt.

Needle/Sample Transport Assembly

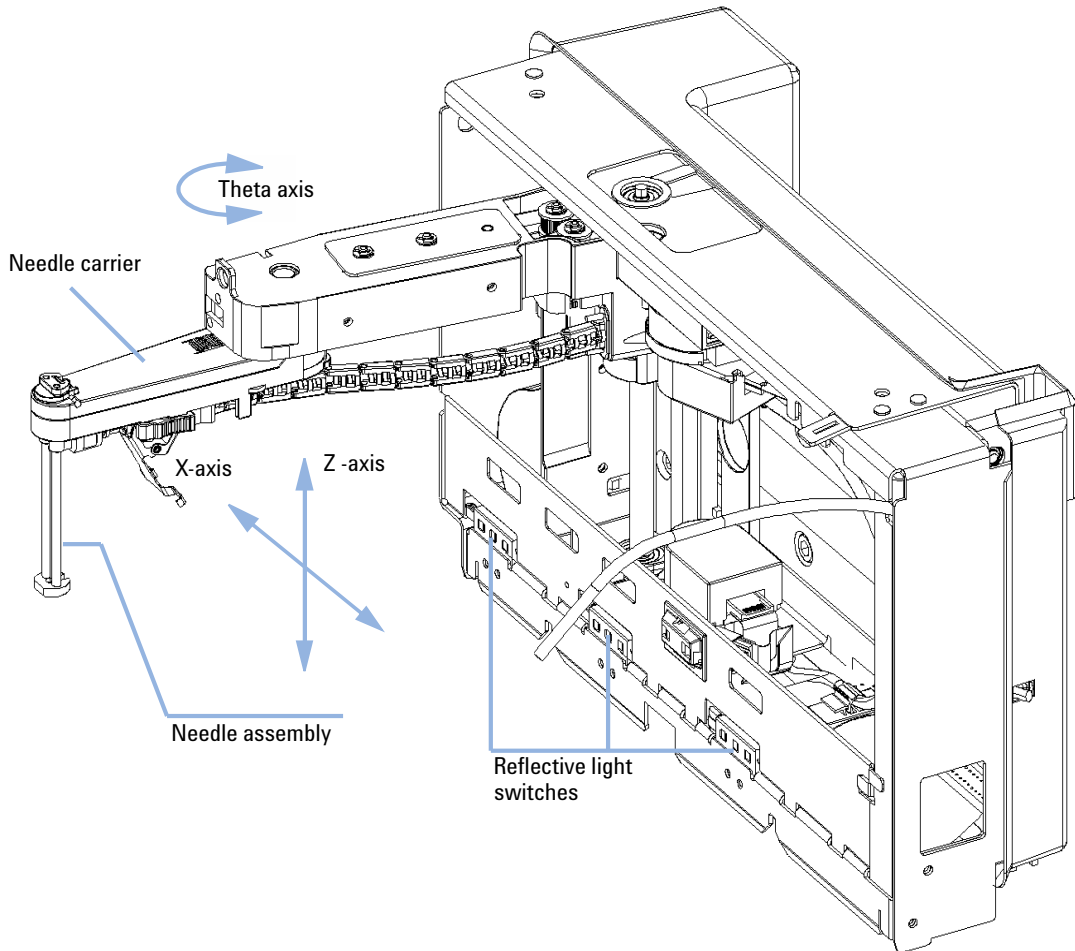


Figure 6 Needle/Sample Transport Assembly

The needle/sample transport is a multifunctional module capable of moving the needle into various positions (such as different wells in two different plates, different vials, needle wash position and the needle-seat position). The active movable axes are the X-axis, the Z-axis and the theta-axis, the vial-/plate pusher is an additional passive axis. All axes are stepper motor driven and encoder controlled in order to have tight feedback for the axes position. The theta and Z axes have spring loaded belt-tensioner.

Reflective light switches detect the presence and type of different trays. The X-slide carries the antenna and electronics of a RF-sensor. This device has multiple functions:

- It allows to read and write information from a tag, located in the new tray.
- It allows to increase the number of different trays.
- It allows to read the revision and other data tags of the needle/sample transport assembly and sampling unit.

Complex flex boards make the electrical connection to the various motors, sensors and the MTP-board. The needle carrier has an integrated plate/vial pusher with an additional linear encoder to sense vials and the presence of plates.

The needle and the loop capillary are user-exchangeable.

The back of the needle/sample transport assembly has a cover to protect the electronics from potential solvent vapor.

Advanced Operating Modes

Multi-Draw Mode (Optional)

The multi-draw mode provides injection volumes up to 1500 µl. In this case a capillary which holds the additional volume is assembled between seat and valve. Then the aspirated sample is pushed into the enlarged seat capillary before repetitive aspiration starts. After the last aspiration took place the injection valve switches and the mobile phase transports sample towards column.

Injector Program

A sequence of all available single sampling steps can be tailored to customer needs for special applications. Injector program capability is offered with the standard instrument

Active Needle Wash

The active needle wash mode allows also the flushing of the outer surface of the needle. This results in an additional decrease of sample carry-over. Duration of the procedure is settable.

Overlap Injection Cycle

Overlapped injection is the mode where the autosampler runs the injector program for the next analysis during the current analysis (without injecting).

After the sample has reached the column the valve is switched back to bypass and the next injection cycle starts but waits with switching to main-pass until the actual run is finished. This mode allows it to increase the sample throughput.

Low Delay Volume Mode

This mode is especially interesting for gradient elution with small bore or capillary columns. The injection valve is switched back to bypass after the sample is eluted beyond the injection valve port # 6. This decreases the delay volume, because the gradient needs not to pass the metering device and the loop capillary.

System Overview

Leak and Waste Handling

The 1200 Infinity Series has been designed for safe leak and waste handling. It is important that all security concepts are understood and instructions are carefully followed.

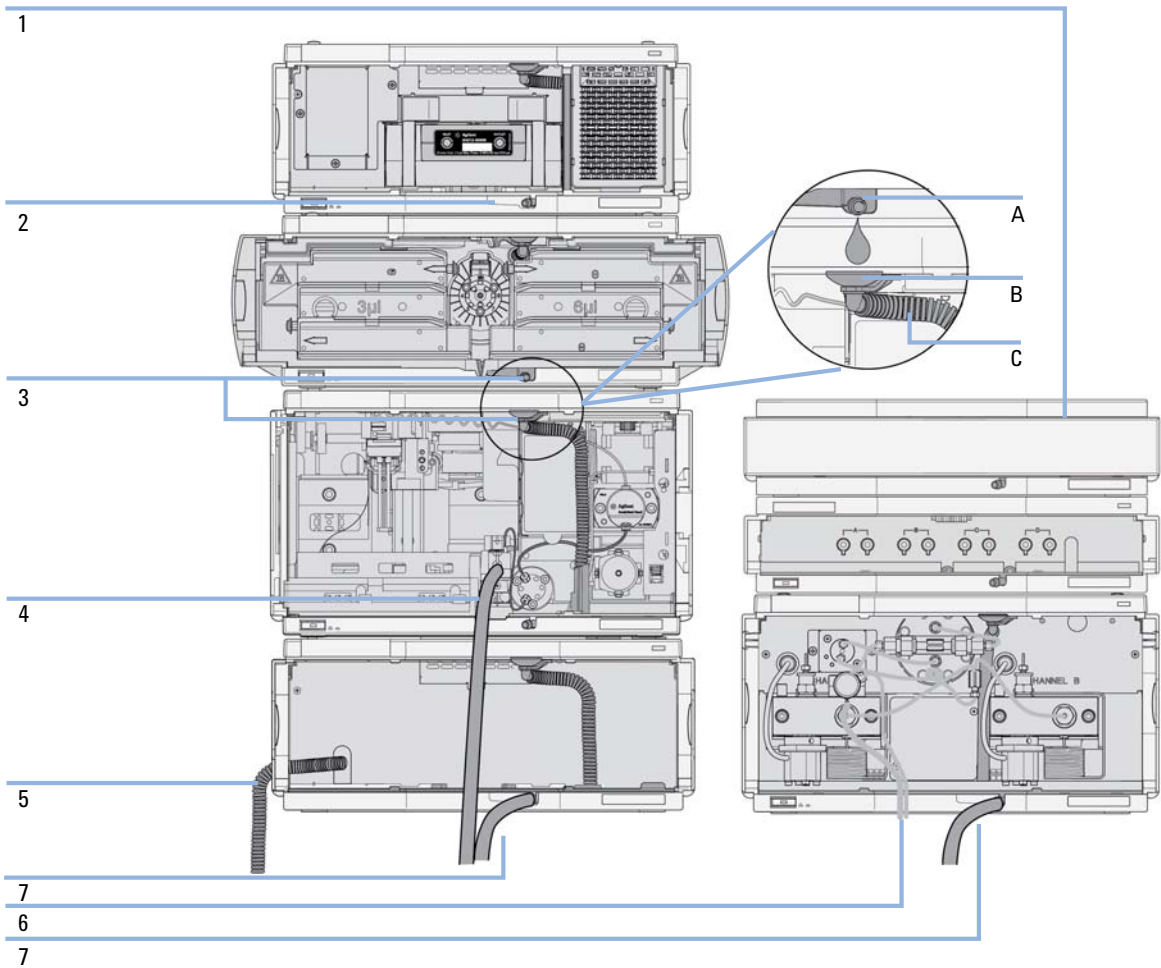


Figure 7 Leak and waste handling concept (overview - typical stack configuration as an example)

The solvent cabinet (1) is designed to store a maximum volume of 6 L solvent. The maximum volume for an individual bottle stored in the solvent cabinet should not exceed 2.5 L. For details, see the usage guideline for the Agilent 1200 Infinity Series Solvent Cabinets (a printed copy of the guideline has been shipped with the solvent cabinet, electronic copies are available on the Internet).

The leak pan (2) (individually designed in each module) guides solvents to the front of the module. The concept covers also leakages on internal parts (e.g. the detector's flow cell). The leak sensor in the leak pan stops the running system as soon as the leak detection level is reached.

The leak pan's outlet port (3, A) guides excessive overflow from one module to the next, as the solvent flows into the next module's leak funnel (3, B) and the connected corrugated waste tube (3, C). The corrugated waste tube guides the solvent to the next lower positioned module's leak tray and sensor.

The waste tube of the sampler's needle wash port (4) guides solvents to waste.

The condense drain outlet of the autosampler cooler (5) guides condensate to waste.

The waste tube of the purge valve (6) guides solvents to waste.

The waste tube connected to the leak pan outlet on each of the bottom instruments (7) guides the solvent to a suitable waste container.

1 Introduction
System Overview



2 Site Requirements and Specifications

Site Requirements	28
Physical Specifications	31
Performance Specifications	32

This chapter describes the site requirements and specifications of the High Performance Micro Autosampler.



Site Requirements

A suitable environment is important to ensure optimal performance of the instrument.

Power Considerations

The module power supply has wide ranging capability. It accepts any line voltage in the range described in [Table 3](#) on page 31. Consequently there is no voltage selector in the rear of the module. There are also no externally accessible fuses, because automatic electronic fuses are implemented in the power supply.

WARNING

Hazard of electrical shock or damage of your instrumentation can result, if the devices are connected to a line voltage higher than specified.

→ Connect your instrument to the specified line voltage only.

WARNING

The module is partially energized when switched off, as long as the power cord is plugged in.

Repair work at the module can lead to personal injuries, e.g. electrical shock, when the cover is opened and the module is connected to power.

→ Always unplug the power cable before opening the cover.

→ Do not connect the power cable to the instrument while the covers are removed.

CAUTION

Inaccessible power plug.

In case of emergency it must be possible to disconnect the instrument from the power line at any time.

→ Make sure the power connector of the instrument can be easily reached and unplugged.

→ Provide sufficient space behind the power socket of the instrument to unplug the cable.

Power Cords

Different power cords are offered as options with the module. The female end of all power cords is identical. It plugs into the power-input socket at the rear. The male end of each power cord is different and designed to match the wall socket of a particular country or region.

WARNING

Absence of ground connection or use of unspecified power cord

The absence of ground connection or the use of unspecified power cord can lead to electric shock or short circuit.

- Never operate your instrumentation from a power outlet that has no ground connection.
 - Never use a power cord other than the Agilent Technologies power cord designed for your region.
-

WARNING

Use of unsupplied cables

Using cables not supplied by Agilent Technologies can lead to damage of the electronic components or personal injury.

- Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.
-

WARNING

Unintended use of supplied power cords

Using power cords for unintended purposes can lead to personal injury or damage of electronic equipment.

- Never use the power cords that Agilent Technologies supplies with this instrument for any other equipment.
-

Bench Space

The module dimensions and weight (see [Table 3](#) on page 31) allow you to place the module on almost any desk or laboratory bench. It needs an additional 2.5 cm (1.0 inches) of space on either side and approximately 8 cm (3.1 inches) in the rear for air circulation and electric connections.

If the bench shall carry a complete HPLC system, make sure that the bench is designed to bear the weight of all modules.

The module should be operated in a horizontal position.

Condensation

CAUTION

Condensation within the module

Condensation will damage the system electronics.

- Do not store, ship or use your module under conditions where temperature fluctuations could cause condensation within the module.
 - If your module was shipped in cold weather, leave it in its box and allow it to warm slowly to room temperature to avoid condensation.
-

Physical Specifications

Table 3 Physical Specifications

Type	Specification	Comments
Weight	15.5 kg (35 lbs)	
Dimensions (height × width × depth)	200 × 345 × 440 mm (8 × 13.5 × 17 inches)	
Line voltage	100 – 240 VAC, ± 10 %	Wide-ranging capability
Line frequency	50 or 60 Hz, ± 5 %	
Power consumption	300 VA / 200 W / 683 BTU	Maximum
Ambient operating temperature	4 – 55 °C (39 – 131 °F)	
Ambient non-operating temperature	-40 – 70 °C (-40 – 158 °F)	
Humidity	< 95 % r.h. at 40 °C (104 °F)	Non-condensing
Operating altitude	Up to 2000 m (6562 ft)	
Non-operating altitude	Up to 4600 m (15091 ft)	For storing the module
Safety standards: IEC, CSA, UL	Installation category II, Pollution degree 2	For indoor use only.

Performance Specifications

Table 4 Performance Specifications

Type	Specification
GLP features	Early maintenance feedback (EMF), electronic records of maintenance and errors
Communications	Controller-area network (CAN). RS232C, APG-remote standard, optional four external contact closures and BCD vial number output
Safety features	Leak detection and safe leak handling, low voltages in maintenance areas, error detection and display
Injection range	0.01 – 8 µL in 0.01 µL increments with the small loop capillary 0.01 – 40 µL in 0.01 µL increments with the extended loop capillary
Precision	Typically < 0.5 % RSD of peak areas from 5 – 40 µL Typically < 1 % RSD from 1 – 5 µL Typically < 3 % RSD from 0.2 – 1 µL
Pressure range	Up to 400 bar (5880 psi)
Sample viscosity range	0.2 – 5 cp
Sample capacity	2 × well-plates (MTP) + 10 × 2 mL vials 108 × 2 mL vials in 2 × 54 vial plate plus 10 additional 2 mL vials 30 × 6 mL vials in 2 × 15 vial plate plus 10 additional 2 mL vials 54 Eppendorf tubes (0.5 /1.5 /2 mL) in 2 × 27 Eppendorf tube plate
Injection cycle time	Typically < 30 s using following standard conditions: <ul style="list-style-type: none"> • Default draw speed: 4 µL/min • Default eject speed: 10 µL/min • Injection volume: 0.1 µL
Carry-over	Typically < 0.05 % using the following conditions: <ul style="list-style-type: none"> • Column: 150 × 0.5 mm Hypersil ODS, 3 µm • Mobile phase: Water/Acetonitrile = 85 /15 • Column Flow rate: 13 µL/min • Injection volume: 1 µL caffeine (=25 ng caffeine), 1 µL water to test carryover • Outside wash of needle before injection: 20 s with water using flush port



3 Installing the Autosampler

Unpacking the Sampler	34
Damaged Packaging	34
Delivery Checklist	34
Accessory Kits	35
Optimizing the Stack Configuration	36
One Stack Configuration	37
Two Stack Configuration	39
Installation Information on Leak and Waste Handling	41
Installing the Autosampler	45
Installing a Thermostatted Autosampler	48
Flow Connections to the Sampler	52
Installing the Sample Tray	54
Transporting the Sampler	56

This chapter describes the installation of the High Performance Micro Autosampler.



Unpacking the Sampler

NOTE

If you need to ship the autosampler at a later date, always use the shipping protection foam parts (see “[Transporting the Sampler](#)” on page 56).

Damaged Packaging

Upon receipt of your module, inspect the shipping containers for any signs of damage. If the containers or cushioning material are damaged, save them until the contents have been checked for completeness and the instrument has been mechanically and electrically checked. If the shipping container or cushioning material is damaged, notify the carrier and save the shipping material for the carrier’s inspection.

Delivery Checklist

Ensure all parts and materials have been delivered with the autosampler. For this compare the shipment content with the checklist included in each instrument box. Please report missing or damaged parts to your local Agilent Technologies sales and service office.

Accessory Kits

p/n	Description
5063-6527	Tubing assembly, i.d. 6 mm, o.d. 9 mm, 1.2 m (to waste)
9222-0518	Bag - plastics
G1315-45003	Torque adapter
G1367-60006	WPS Leak Kit
G1375-87304	Fused silica/PEEK capillary 50 μ m, 50 cm
G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat
G1329-43200	Adapter air channel
5181-1519	CAN cable, Agilent module to module, 1 m
8710-1534	Wrench, 4 mm both ends, open end
G1377-44900	tool for Micro Seat Capillary Mounting
G1377-87300	Loop capillary, 40 μ L for G1377A

Optimizing the Stack Configuration

If your module is part of a complete Agilent Liquid Chromatograph, you can ensure optimum performance by installing the following configurations. These configurations optimize the system flow path, ensuring minimum delay volume.

One Stack Configuration

Ensure optimum performance by installing the modules of the Agilent 1260 Infinity LC System in the following configuration (See [Figure 8](#) on page 37 and [Figure 9](#) on page 38). This configuration optimizes the flow path for minimum delay volume and minimizes the bench space required.

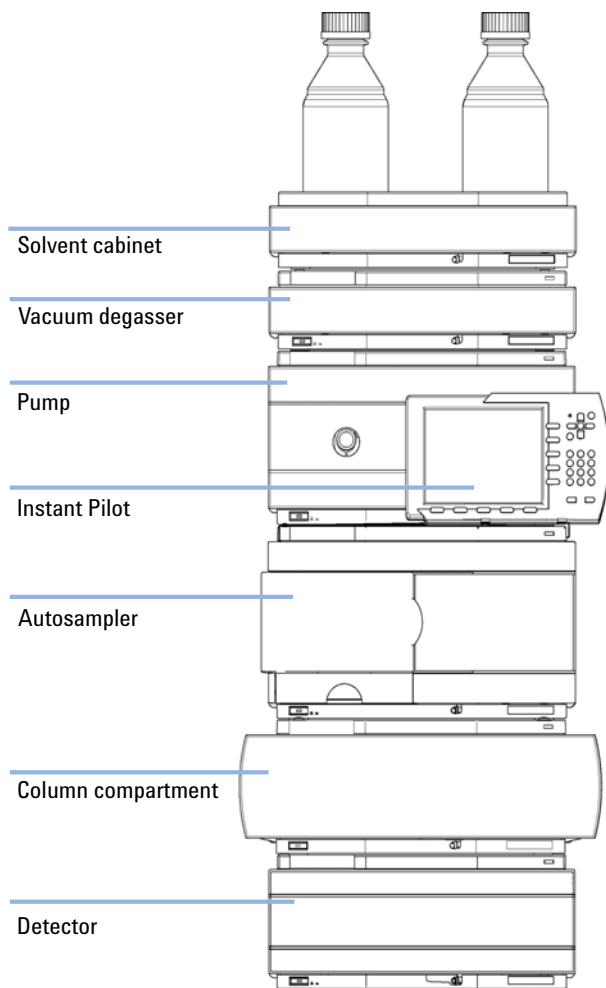


Figure 8 Recommended Stack Configuration for 1260 Infinity (Front View)

3 Installing the Autosampler

Optimizing the Stack Configuration

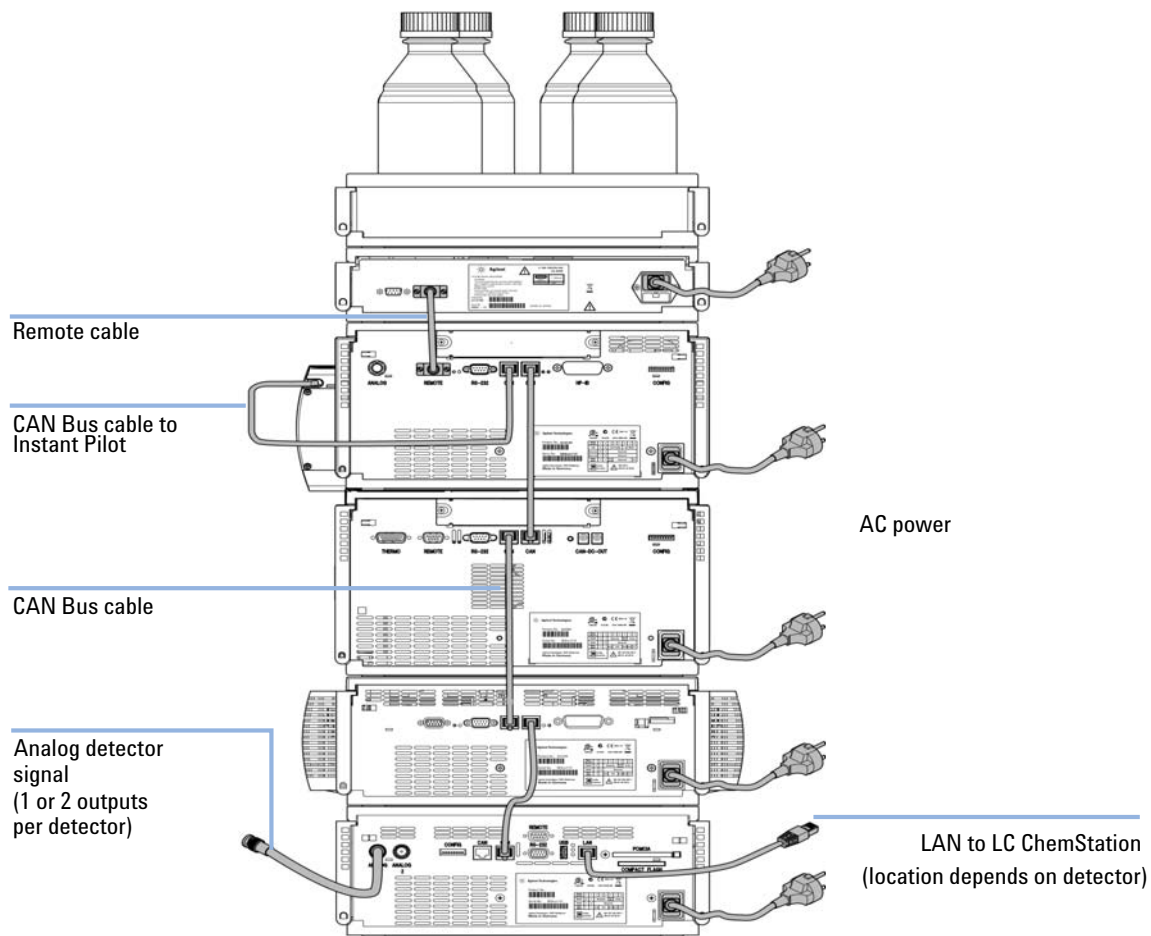


Figure 9 Recommended Stack Configuration for 1260 Infinity (Rear View)

Two Stack Configuration

To avoid excessive height of the stack when the autosampler thermostat is added to the system it is recommended to form two stacks. Some users prefer the lower height of this arrangement even without the autosampler thermostat. A slightly longer capillary is required between the pump and autosampler. (See [Figure 10](#) on page 39 and [Figure 11](#) on page 40).

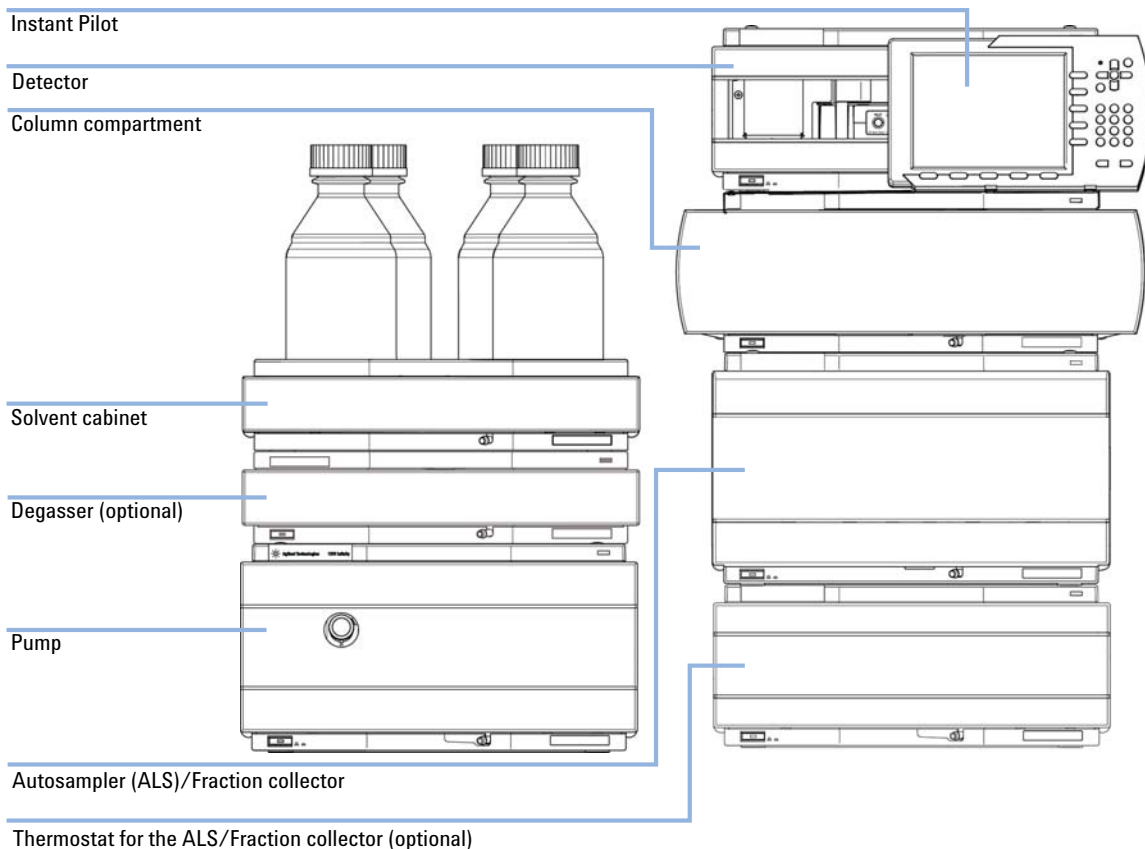


Figure 10 Recommended Two Stack Configuration for 1260 Infinity (Front View)

3 Installing the Autosampler Optimizing the Stack Configuration

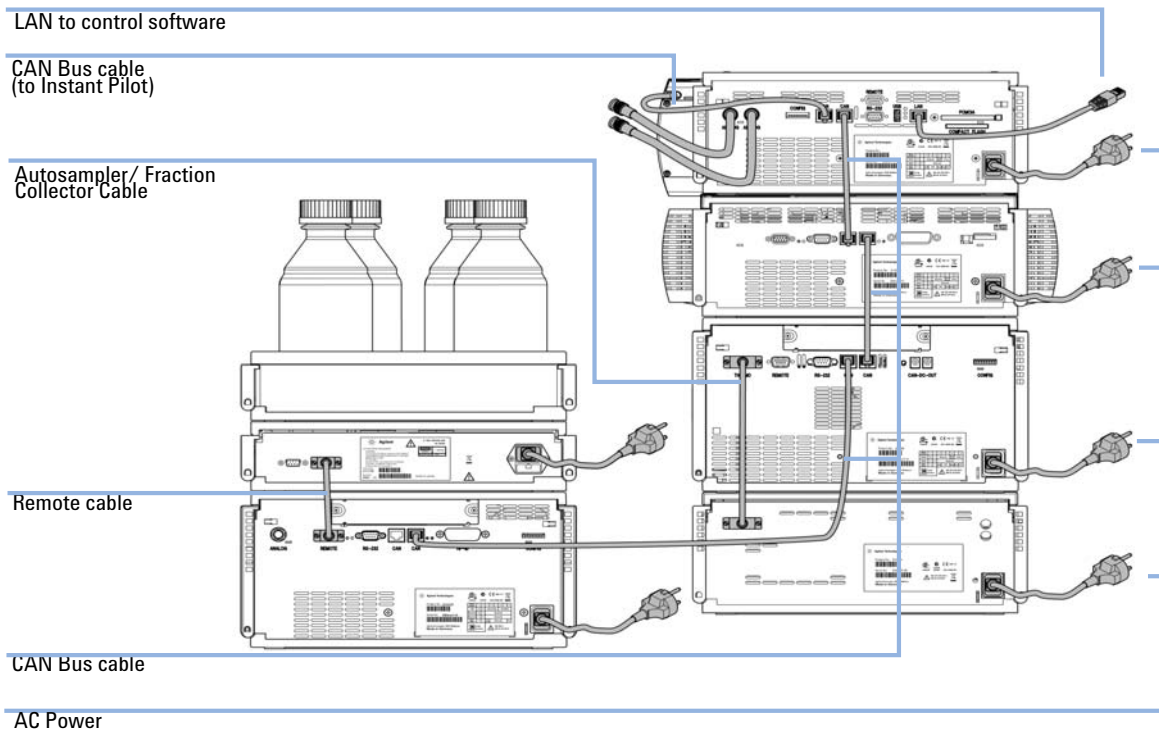


Figure 11 Recommended Two Stack Configuration for 1260 Infinity (Rear View)

Installation Information on Leak and Waste Handling

The Agilent 1200 Infinity Series has been designed for safe leak and waste handling. It is important that all security concepts are understood and instructions are carefully followed.

WARNING

Toxic, flammable and hazardous solvents, samples and reagents

The handling of solvents, samples and reagents can hold health and safety risks.

- When working with these substances observe appropriate safety procedures (for example by wearing goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the vendor, and follow good laboratory practice.
- The volume of substances should be reduced to the minimum required for the analysis.
- Never exceed the maximal permissible volume of solvents (6 L) in the solvent cabinet.
- Do not use bottles that exceed the maximum permissible volume as specified in the usage guideline for the Agilent 1200 Infinity Series Solvent Cabinets.
- Arrange the bottles as specified in the usage guideline for the solvent cabinet.
- A printed copy of the guideline has been shipped with the solvent cabinet, electronic copies are available on the Internet.

NOTE

Recommendations for Solvent Cabinet

For details, see the usage guideline for the Agilent 1200 Infinity Series Solvent Cabinets.

3 Installing the Autosampler

Installation Information on Leak and Waste Handling

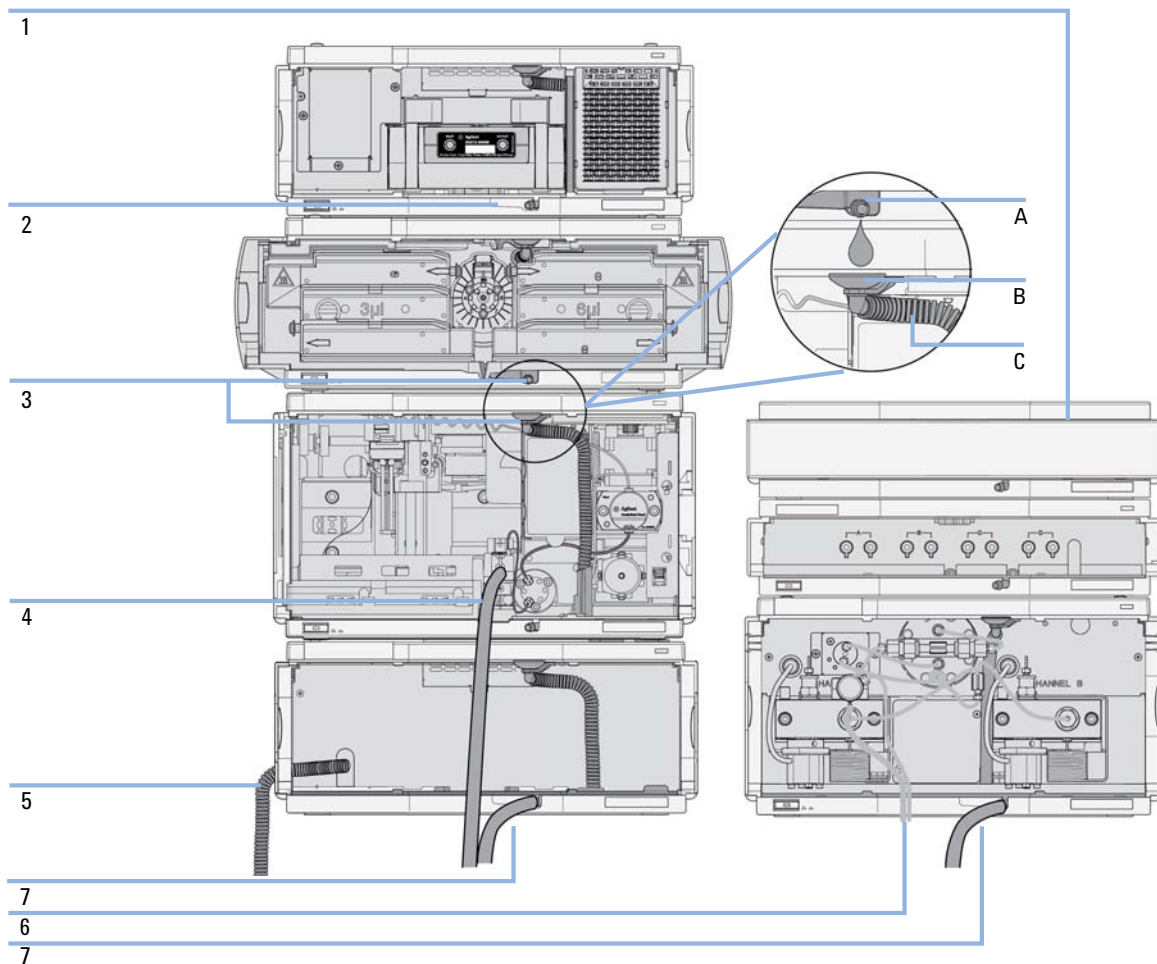


Figure 12 Leak and waste handling (overview - typical stack configuration as an example)

1	Solvent cabinet
2	Leak pan
3	Leak pan's outlet port (A), leak funnel (B) and corrugated waste tube (C)
4	Waste tube of the sampler's needle wash
5	Condense drain outlet of the autosampler cooler
6	Waste tube of the purge valve
7	Waste tube

- 1 Stack the modules according to the adequate stack configuration.
The leak pan outlet of the upper module must be vertically positioned above the leak tray of the lower module, see [Figure 12](#) on page 42.
- 2 Connect data and power cables to the modules, see section *Installing the Module* below.
- 3 Connect capillaries and tubes to the modules, see section *Flow Connections to the module* below or the relevant system manual.

WARNING

Toxic, flammable and hazardous solvents, samples and reagents

- Keep solvent path free from blockages.
- Keep the flow path closed (in case the pump in the system is equipped with a passive inlet valve, solvent may leak out due to hydrostatic pressure, even if your instrument is off).
- Avoid loops.
- Tubes must not sag.
- Do not bend tubes.
- Do not immerse tube end in waste liquid.
- Do not intubate tubes in other tubes.
- For correct tubing follow instructions on label attached to the module.

3 Installing the Autosampler

Installation Information on Leak and Waste Handling



Figure 13 Warning label (illustration for correct waste tubing)

Installing the Autosampler

Parts required	#	Description
	1	Sampler Power cord.

Preparations

- Locate bench space Provide power connections Unpack the sampler

WARNING

Instruments are partially energized when switched off

The power supplies still use some power, even if the power switch on the front panel is turned off.

- To disconnect the thermostatted autosampler from line power, unplug the power cord from the autosampler and the ALS thermostat.
 - Make sure that it is always possible to access the power plug.
-

WARNING

Personal injury

To avoid personal injury, keep fingers away from the needle area during autosampler operation.

- Do not attempt to insert or remove a vial or a plate when the needle is positioned.
-

CAUTION

"Defective on arrival" problems

If there are signs of damage, please do not attempt to install the module. Inspection by Agilent is required to evaluate if the instrument is in good condition or damaged.

- Notify your Agilent sales and service office about the damage.
 - An Agilent service representative will inspect the instrument at your site and initiate appropriate actions.
-

3 Installing the Autosampler

Installing the Autosampler

- 1** Install the LAN interface board in the sampler (if required).
- 2** Remove the adhesive tape which covers the side and front doors.
- 3** Open the front door and remove the left side door.
- 4** Remove the transport protection foam.
- 5** Re-install the corrugated waste tube in the plastic port.
- 6** Re-install the left side door (take care of the magnet at the back).
- 7** Place the autosampler in the stack or on the bench in all horizontal position.
- 8** Ensure the power switch at the front of the sampler is OFF.
- 9** Connect the power cable to the power connector at the rear of the sampler.
- 10** Connect the CAN cable to the other Agilent modules.
- 11** If a Agilent ChemStation is the controller, connect the LAN connection to the LAN interface
- 12** Connect the APG remote cable (optional) for non Agilent 1200 Infinity Series instruments.
- 13** Ensure the side panel is correctly installed.
- 14** Turn ON power by pushing the button at the lower left hand side of the sampler.
- 15** Close the front door. The exhaust fan will turn ON and remove the vapor from the tray compartment. After 1-2 minutes the sampler will

start the hardware initialisation process. At the end of this process the status LED should be off.

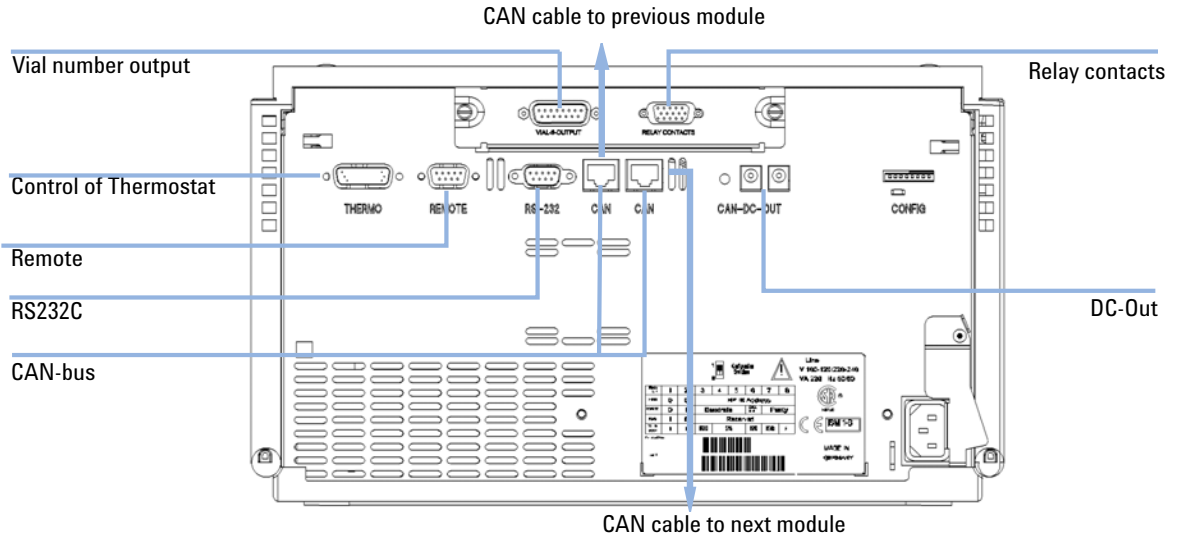


Figure 14 Cable Connections

NOTE

The sampler is turned ON when the line power switch is pressed and the green indicator lamp is illuminated. The sampler is turned OFF when the line power switch is protruding and the green light is OFF.

Installing a Thermostatted Autosampler

Parts required	#	Description
	1	Sampler and thermostat Power cord.

Preparations

- Locate bench space Provide power connections Unpack the sampler and the thermostat

WARNING

Instrument is partially energized when switched off

The power supply still uses some power, even if the power switch at the front of the panel is turned off.

→ To disconnect the sampler from the line, unplug the power cord.

CAUTION

Damaged electronics

Disconnecting or reconnecting the sampler to thermostat cable when the power cords are connected to either of the two modules will damage the electronics of the modules.

→ Make sure the power cords are unplugged before disconnecting or reconnecting the sampler to thermostat cable.

CAUTION

Damage through condensation

If the condensation tube is located in liquid the condensed water cannot flow out of the tube and the outlet is blocked. Any further condensation will then remain in the instrument. This may damage the instruments electronics.

→ Make sure the condensation tube is always above the liquid level in the vessel.

→ Make sure the waste container is not sealed.

→ Ensure the drain tube has no loops and leads directly into the waste bottle.

WARNING

Personal injury

To avoid personal injury, keep fingers away from the needle area during autosampler operation.

→ Do not attempt to insert or remove a vial or a plate when the needle is positioned.

- 1 Place the thermostat on the bench.
- 2 Remove the front cover and route the condensation drain tube to the waste bottle.

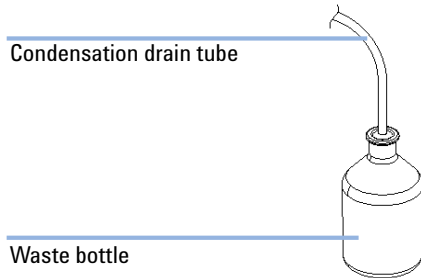


Figure 15 Condensation leak outlet

- 3 Install the LAN interface board in the sampler (if required).
- 4 Remove the adhesive tape which covers the side and front doors.
- 5 Open the front door and remove the left side door.
- 6 Remove the transport protection foam.
- 7 Re-install the corrugated waste tube in the plastic port.
- 8 Re-install the left side door (take care of the magnet at the back).
- 9 Place the sampler on top of the thermostat. Make sure that the sampler is correctly engaged in the thermostat locks.

3 Installing the Autosampler

Installing a Thermostatted Autosampler

- 10 Remove the tray and the plastic cover from the tray base, place the air channel adapter into the sampler tray base. Make sure the adapter is fully pressed down. This assures that the cold airstream from the thermostat is correctly guided to the tray area of the well plate sampler.

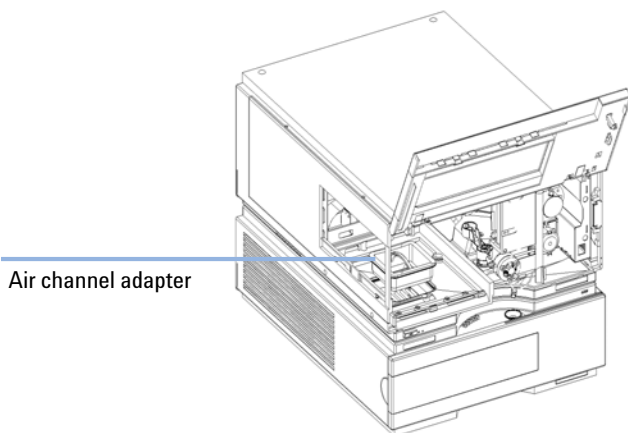


Figure 16 Installation of Thermostat and Autosampler

- 11 Re-install the tray.
- 12 Ensure the power switch on the front of the sampler is OFF and the power cables are disconnected.
- 13 Connect the cable between the sampler and the thermostat, see [Figure 17](#) on page 51.
- 14 Connect the power cables to the power connectors.
- 15 Connect the CAN cable to other Agilent modules.
- 16 If a Agilent ChemStation is the controller, connect the LAN connection to the LAN interface
- 17 Connect the APG remote cable (optional) for non Agilent 1200 Infinity Series instruments.
- 18 Ensure the side panel is correctly installed.
- 19 Turn ON power by pushing the button at the lower left hand side of the sampler.
- 20 Close the front door.

The exhaust fan will turn ON and remove the vapor from the tray compartment. After 1-2 minutes the sampler will start tile hardware initialisation process. At the end of this process the status LED should be off.

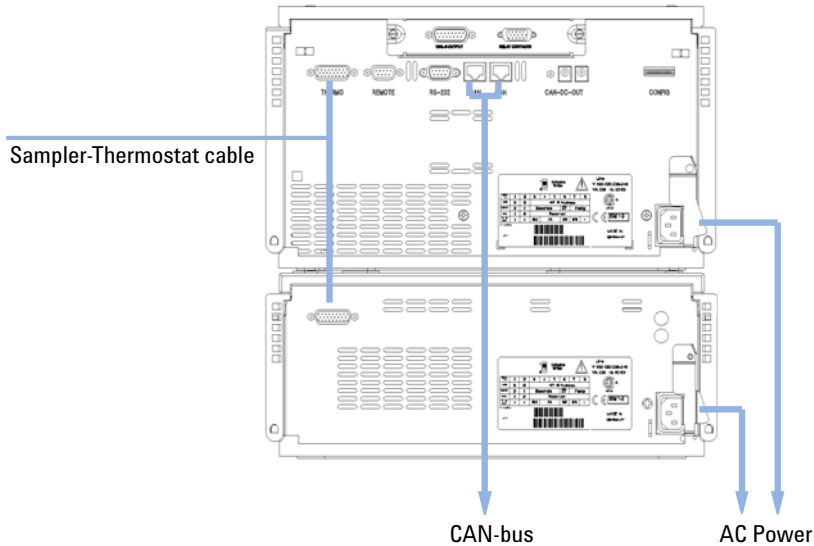


Figure 17 Connection at the rear of thermostatted Autosampler

NOTE

The sampler is turned ON when the line power switch is pressed and the green indicator lamp is illuminated. The sampler is turned OFF when the line power switch is protruding and the green light is OFF.

Flow Connections to the Sampler

Parts required	#	Description
	1	Parts from the accessory kits, see “Accessory Kits” on page 35

Preparations

- Sampler is installed in the LC system

WARNING

When opening capillary or tube fittings, solvents may leak out.

The handling of toxic and hazardous solvents and reagents can carry health risks.

→ Observe appropriate safety procedures (for example, wear goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the solvent vendor, especially when toxic or hazardous solvents are used.

-
- 1 Connect the pump outlet capillary to port 1 of the injection valve.
 - 2 Connect column-compartment inlet capillary to port 6 of the injection valve.
 - 3 Connect the corrugated waste tube to the seat adapter and the solvent waste from the leak plane.
 - 4 Ensure that the waste tube is positioned inside the leak channel.
 - 5 Drive the tube from the peristaltic flush pump to the solvent bottle in the solvent cabinet

- 6 Seat capillary: see recommendations in “Choice of Seat Capillary” on page 83

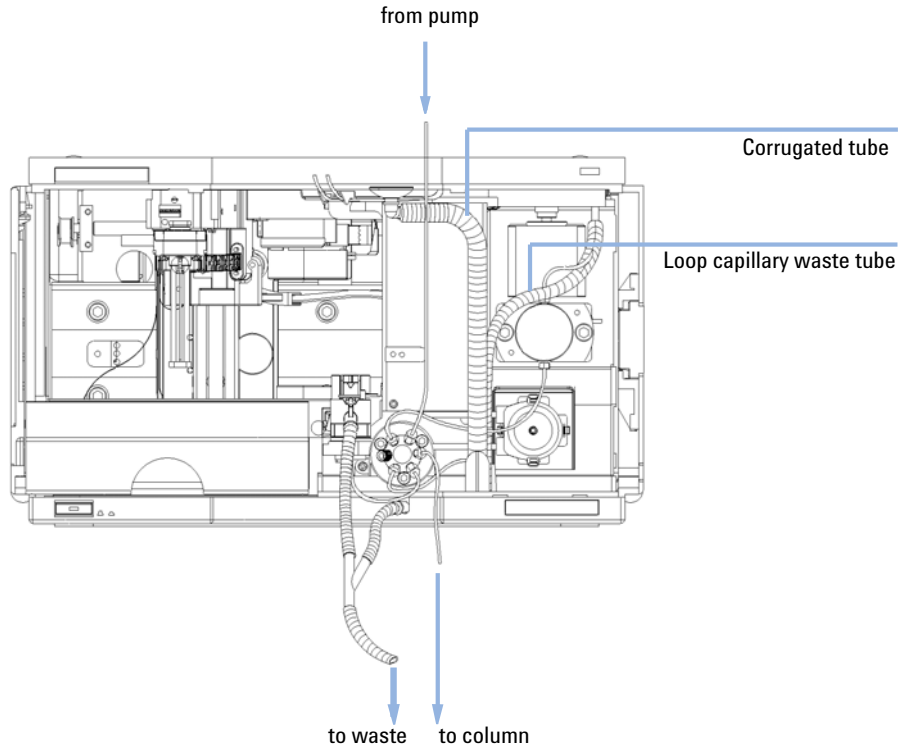


Figure 18 Hydraulic Connections

Installing the Sample Tray

- 1 Press the bottom on the right side to release the front door.
- 2 Lift the front door.
- 3 Load the sample tray with sample well plates and vials as required.
- 4 Slide the sample tray into the autosampler so that the rear of the sample tray is seated firmly against the rear of the sample-tray area.
- 5 Press the front of the sample tray down to secure the tray in the autosampler.

NOTE

If the tray pops out of position the air channel adapter is not correctly inserted.

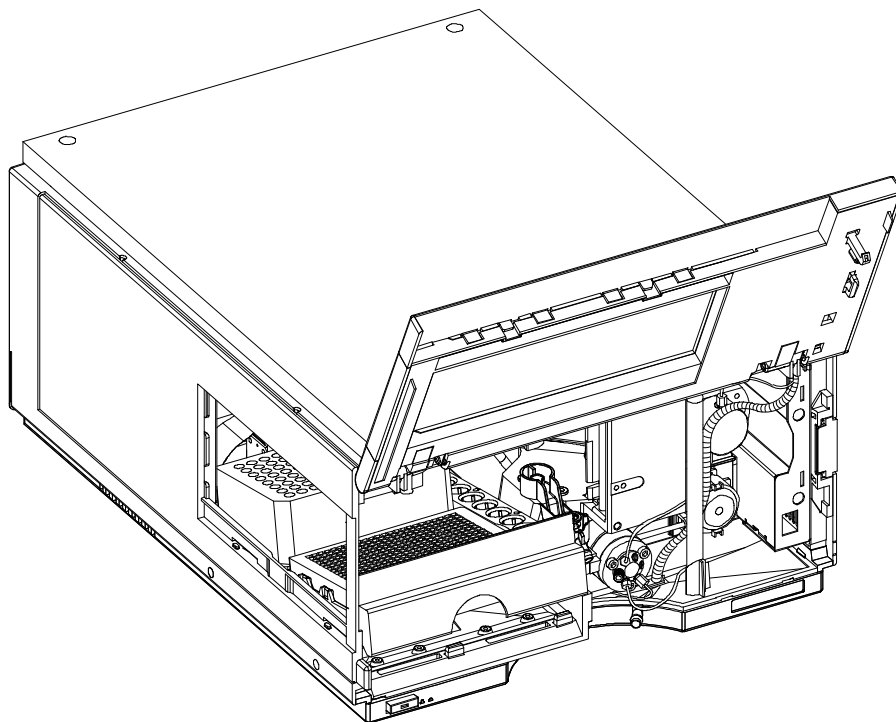


Figure 19 Installing the Sample Tray

Transporting the Sampler

When moving the autosampler inside the laboratory, no special precautions are needed. However, if the autosampler needs to be shipped to another location via carrier, ensure:

- The transport assembly is in the park position. Use the Lab Monitor and Diagnostic software or the Instant Pilot for this command.
- The vial tray and the sample transport mechanism is secured with the transport protection foam.



4 Using the Autosampler

Leak and Waste Handling	58
Sample Trays	59
List of Recommended Plates and Closing Mat	60
List of Recommended Vials and Caps	62
Configure Well Plate Types	64
Turn ON and Initialization Steps	67

This chapter describes the usage of the High Performance Micro Autosampler.



Leak and Waste Handling

WARNING

Toxic, flammable and hazardous solvents, samples and reagents

The handling of solvents, samples and reagents can hold health and safety risks.

- When working with these substances observe appropriate safety procedures (for example by wearing goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the vendor, and follow good laboratory practice.
- The volume of substances should be reduced to the minimum required for the analysis.
- Do not operate the instrument in an explosive atmosphere.
- Never exceed the maximal permissible volume of solvents (6 L) in the solvent cabinet.
- Do not use bottles that exceed the maximum permissible volume as specified in the usage guideline for the Agilent 1200 Infinity Series Solvent Cabinets.
- Arrange the bottles as specified in the usage guideline for the solvent cabinet.
- A printed copy of the guideline has been shipped with the solvent cabinet, electronic copies are available on the Internet.
- The residual free volume in the appropriate waste container must be large enough to collect the waste liquid.
- Check the filling level of the waste container regularly.
- To achieve maximal safety, check the correct installation regularly.

NOTE

Recommendations for Solvent Cabinet

For details, see the usage guideline for the Agilent 1200 Infinity Series Solvent Cabinets.

For details on correct installation, see [“Installation Information on Leak and Waste Handling”](#) on page 41.

Sample Trays

Supported Trays for an Autosampler

Table 5 Trays for an Autosampler

G2258-60011	Tray for 2 well plates or vial plates and 10 x 2 ml vials
-------------	---

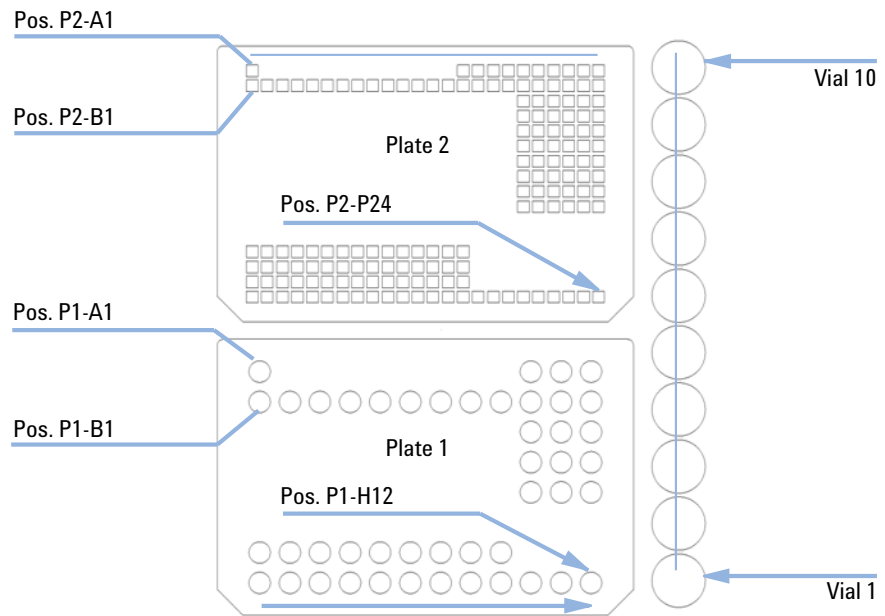


Figure 20 Numbering of vial and well plate position

List of Recommended Plates and Closing Mat

WARNING

Explosive gas mixtures

There is a risk of building explosive gas mixtures in the instrument if flammable solvents are used.

- Cover the plates.
 - Remove the plates from the sampler after turning it OFF.
-

WARNING

Contamination with adhesives

Closing mats with adhesive can give some contamination in the system. The adhesive is soluble in most of the solvents used in HPLC.

- In general do not use closing mats with adhesive. The sampler has no prepunch needle, therefore the adhesive will clog the needle after several injections.
-

Table 6 Recommended plates and closing mat

Description	Rows	Columns	Plate height	Volume (µl)	Part Number	Package
384Agilent	16	24	14.4	80	p/n 5042-1388	30
384Corning	16	24	14.4	80	No Agilent PN	
384Nunc	16	24	14.4	80	No Agilent PN	
96Agilent	8	12	14.3	400	p/n 5042-1386 p/n 5042-1385	10 120
96Agilent conical	8	12	17.3	150	p/n 5042-8502	25
96CappedAgilent	8	12	47.1	300	p/n 5065-4402	1
96Corning	8	12	14.3	300	No Agilent PN	
96CorningV	8	12	14.3	300	No Agilent PN	
96DeepAgilent31mm	8	12	31.5	1000	p/n 5042-6454	50
96DeepNunc31mm	8	12	31.5	1000	No Agilent PN	
96DeepRitter41mm	8	12	41.2	800	No Agilent PN	
96Greiner	8	12	14.3	300	No Agilent PN	
96GreinerV	8	12	14.3	250	No Agilent PN	
96Nunc	8	12	14.3	400	No Agilent PN	
Closing mat for all 96 Agilent plates	8	12			p/n 5042-1389	50

Table 7 Recommended Vial plates

Description	Part Number
• Vial plate for 54 x 2 ml vials (6/pk)	p/n G2255-68700
• Vial plate for 15 x 6 ml vials (1/pk)	p/n 5022-6539
• Vial Plate for 27 Eppendorf tubes	p/n 5022-6538

List of Recommended Vials and Caps

Table 8 Crimp Top Vials

Description	Volume (ml)	100/Pack	1000/Pack	100/Pack (silanized)
Clear glass	2	p/n 5181-3375	p/n 5183-4491	
Clear glass, write-on spot	2	p/n 5182-0543	p/n 5183-4492	p/n 5183-4494
Amber glass, write-on spot	2	p/n 5182-3376	p/n 5183-4493	p/n 5183-4495

Table 9 SnapTop Vials

Description	Volume (ml)	100/Pack	1000/Pack	100/Pack (silanized)
Clear glass	2	p/n 5182-0544	p/n 5183-4504	p/n 5183-4507
Clear glass, write-on spot	2	p/n 5182-0546	p/n 5183-4505	p/n 5183-4508
Amber glass, write-on spot	2	p/n 5182-0545	p/n 5183-4506	p/n 5183-4509

Table 10 Screw Top Vials

Description	Volume (ml)	100/Pack	1000/Pack	100/Pack (silanized)
Clear glass	2	p/n 5182-0714	p/n 5183-2067	p/n 5183-2070
Clear glass, write-on spot	2	p/n 5182-0715	p/n 5183-2068	p/n 5183-2071
Amber glass, write-on spot	2	p/n 5182-0716	p/n 5183-2069	p/n 5183-2072

Table 11 Crimp Caps

Description	Septa	100/Pack
Silver aluminum	Clear PTFE/red rubber	p/n 5181-1210
Silver aluminum	Clear PTFE/red rubber	p/n 5183-4498 (1000/Pack)
Blue aluminum	Clear PTFE/red rubber	p/n 5181-1215
Green aluminum	Clear PTFE/red rubber	p/n 5181-1216
Red aluminum	Clear PTFE/red rubber	p/n 5181-1217

Table 12 Snap Caps

Description	Septa	100/Pack
Clear polypropylene	Clear PTFE/red rubber	p/n 5182-0550
Blue polypropylene	Clear PTFE/red rubber	p/n 5182-3458
Green polypropylene	Clear PTFE/red rubber	p/n 5182-3457
Red polypropylene	Clear PTFE/red rubber	p/n 5182-3459

Table 13 Screw Caps

Description	Septa	100/Pack
Blue polypropylene	Clear PTFE/red rubber	p/n 5182-0717
Green polypropylene	Clear PTFE/red rubber	p/n 5182-0718
Red polypropylene	Clear PTFE/red rubber	p/n 5182-0719
Blue polypropylene	Clear PTFE/silicone	p/n 5182-0720
Green polypropylene	Clear PTFE/silicone	p/n 5182-0721
Red polypropylene	Clear PTFE/silicone	p/n 5182-0722

Configure Well Plate Types

If the plate you are using is not found on the “[List of Recommended Plates and Closing Mat](#)” on page 60 you may configure a custom plate. Measure the exact dimensions of the plate as marked below and enter the values in the plate configuration table of the ChemStation.

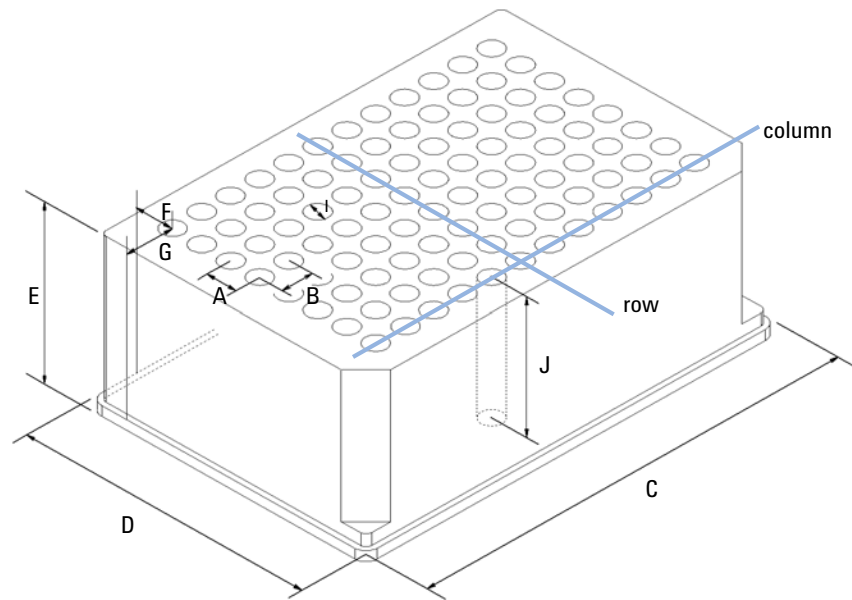


Figure 21 Well Plate Dimensions (straight)

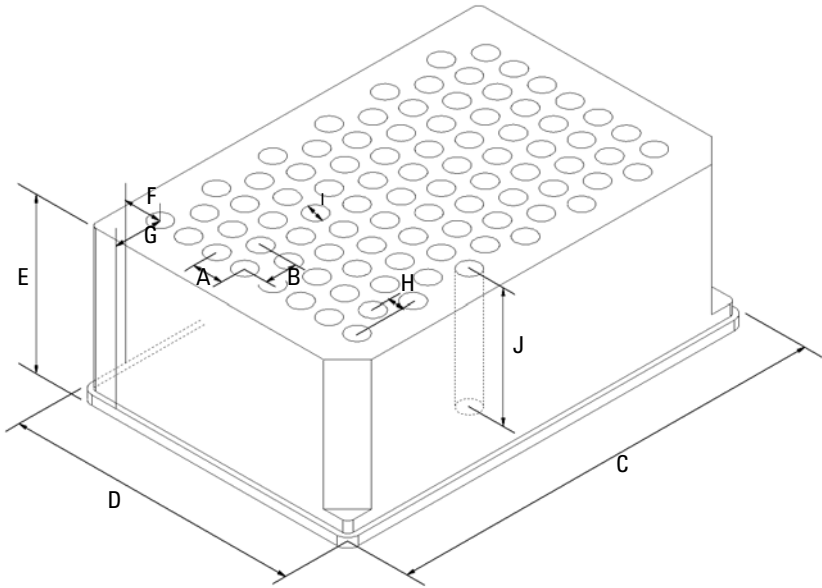


Figure 22 Well Plate Dimensions (staggered)

4 Using the Autosampler

Configure Well Plate Types

Table 14 Well Plate Dimensions

Location	Description	Definition	Limits
	Rows	Number of rows on the plate	up to 16
	Columns	Number of columns on the plate	up to 24
	Volume	Volume (in μl) of a sample vessel	
A	Row distance	Distance (in mm) between the center of two rows	
B	Column distance	Distance (in mm) between the center of two columns	
C	Plate length	X size (in mm) at the bottom of the plate	127.75+/- 0.25 mm (SBS Standard)
D	Plate width	Y size (in mm) at the bottom of the plate	85.50+/-0.25 mm (SBS Standard)
E	Plate height	Size (in mm) from the bottom to the top of the plate	up to 47 mm
F	Row offset	Distance (in mm) from the back edge (bottom) to the center of the first hole (A1)	
G	Column offset	Distance (in mm) from the left edge (bottom) to the center of the first hole (A1)	
H	Column shift	Offset (in mm) to Y when the rows are not straight but staggered	
I	Well diameter	Diameter (in mm) of the well	at least 4 mm
J	Well depth	Distance (in mm) from the top of the plate to the bottom of the well	up to 45 mm

NOTE

The distances need to be measured with high precision. It is recommended to use calipers.

Turn ON and Initialization Steps

A successful turn-on/initialization takes about 3.5 minutes, and consists of five steps

- 1 WPS turn on, begins when the main power button is pushed ON. Power indicator turns green. Front cover latch activates immediately.
- 2 Main fan and exhaust fan turn-on immediately.
- 3 Main board self-test begins. Status indicator tests red, green and yellow, then goes to yellow. This takes about 20 seconds (from turn-on). The status indicator remains yellow until the initialization process is complete. The user interface indicates “initializing” during this period.
- 4 The vapor blowout period begins. This lasts for about 2 minutes.
- 5 WPS sample transport and sampling unit initialization begins at the 2-minutes mark (from turn-on), if the front cover is closed. If the front cover is open at the 2 minutes mark, initialization will start only when the front cover is closed. Initialization takes about 1.5 minutes. When initialization is complete the needle is in the needle seat, the needle lock is down, and the status indicator is off.

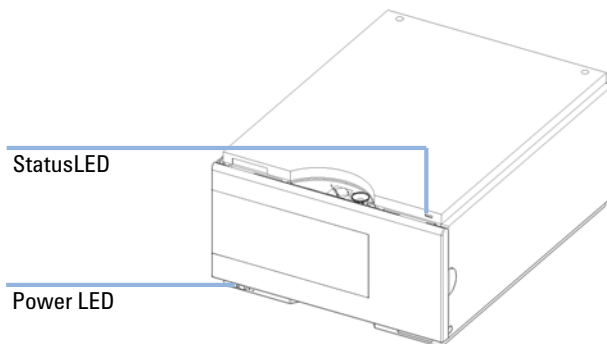


Figure 23 Instrument LED indicator

4 Using the Autosampler

Turn ON and Initialization Steps



5 Optimizing Performance

Optimizing Performance	70
Optimization for Lowest Carry-Over	71
General Recommendations for Lowest Carry-over	72
Specific Recommendations if Bypass Operation is Performed	73
Using the Automated Needle Wash	74
Using the Flush Port	75
Cleaning the needle seat	76
Fast Injection Cycle and Low Delay Volume	78
General Recommendations for Fast Injection Cycle Times	78
Overlapped Injection After Gradient is Flushed Out	79
Overlapped Injection During Run	79
Precise Injection Volume	80
Draw and Eject Speed	80
Choice of Rotor Seal	82
Choice of Seat Capillary	83

This chapter provides information on how to optimize the autosampler.



Optimizing Performance

Autosamplers are more and more used in HPLC to improve the productivity in the laboratories and the consistency and accuracy of analytical results.

The informations below will help you on how to optimize some parameters to achieve best results for:

- lowest carry-over for reliable quantitative data
- Fast injection cycles for high throughput
- Low delay volume for fast gradient
- Precise injection volume

Optimization for Lowest Carry-Over

Carry over (CO) is not only a topic for injection systems but may have multiple sources:

Hardware related

- sample loop
- needle outside
- needle inside
- needle seat
- seat capillary
- injection valve
- flush time
- wash vials
- fittings
- column (carry-over depends on frit design/material/blockage)
- surface activity of frits
- capillaries

Chemistry/Physics related:

- suitable sample solvent (has to be compatible with mobile phase)
- suitable wash solvent
- suitable mobile phase
- column packing material (e.g. interaction of basic sample with silanols of stationary phase)

The autosampler continuous flow-through design ensures that sample loop, needle inside, seat capillary, and the mainpass of the injection valve is always in the flow line. These parts are continuously flushed during an isocratic and also during a gradient analysis. The residual amount of sample remaining on the outside of the needle after injection may contribute to carry-over in some instances. When using small injection volumes or when injecting samples of low concentration immediately after samples of high concentration, carry-over may become noticeable. Cleaning the needle in the flush port or using the automated needle wash enables the carry-over to be minimized and prevents also contamination of the needle seat.

General Recommendations for Lowest Carry-over

Issues in setting up the experiments:

- Use a flush solvent which dissolves the sample well (e.g. aqueous/(organic) acidic for basic samples); set needle wash time to at least 10 sec.
- Use a sample solvent which is compatible with sample and mobile phase. Organic sample solvents (e.g. DMSO) injected into aqueous mobile phase often cause samples to partially deposit on surfaces causing high carry-over. Chlorhexidine, for example, dissolved as a free base in methanol and injected into an acidic aqueous mobile phase shows increased carryover than if it is dissolved in 0.1% TFA. Since it dissolves slowly (but well) in acidic aqueous solvents, it partially deposits on surfaces during the injection cycle.
- Take care at loop capillary change: Push loop capillary forward when tightening the fitting to the needle, ensuring gapless transition from loop to needle. A replaced needle-seat-pair may need 100-200 injections for best carry-over results

Routinely work:

- Prime flush pump for 30 sec. with appropriate solvent previous to the first run after usage outage.
- Ensure that the needle seat is not contaminated. For cleaning the needle seat see chapter “Cleaning the needle seat”.
- Use mainpass operation to avoid discrimination of samples.
- Notice backpressure of a new column; an increase of 10% over time may cause an 10 fold increase in carry-over due to the column.
- Blank vials can be used at least 30 injections.

Specific Recommendations if Bypass Operation is Performed

Bypass operation can severely impact carry-over performance due to the fact that during gradient operation the sample path is not flushed with organic mobile phase. This may cause sample discrimination and/or adsorption of especially lipophilic components in loop, needle and seat flow path.

The term bypass operation in this context describes all cases where the Autosampler is switched to the “Bypass Mode” so that the exposure of the Autosampler’s internal flow path parts to the solvent flow coming from the pump may become too short. This may be the case:

- when overlapped Injection with option “when sample is flushed out” is selected
- when the delay volume is minimized by using “Automated Delay Volume Reduction”

This mode is not recommended as there may arise two sources for carry-over. The outlet groove of the injection valve may be contaminated with sample. This is the minor issue and can be resolved by performing steps for cleaning the injection valve (by method or by injector program). The much more problematic issue is that there may remain portions of sample in the sampler. Especially if the sample and sample solvent doesn’t fit to the mobile phase an arbitrarily large amount of sample may miss the column but stay in the main pass. The “Injector Purge Kit” was developed for this purpose. During run the syringe is used as purge pump and afterwards exchanges the purge solvent with (gradient) start conditions. Using this kit decreases the poor bypass carry-over significantly. Eventually main pass performance may be obtained. But the kit does not resolve the problem of discriminating sample compounds.

Contraindication for usage:

- If run times are below 2-3min the purge kit won’t help as the purge step with reasonable purge volume lasts at least 2min.
- In highly carry-over sensitive applications purge kit is not recommended as best performance is got when the Autosampler stays in mainpass the full solvent gradient.

Control software support for the Purge kit is provided and fully operated and controlled through the ChemStation or and G4208A Instant Pilot via the Autosampler Settings (Requires Agilent ChemStation B.01.03 or higher and Firmware A.06.01 and higher on ALL Agilent 1260 Infinity modules that are part of the system).

Using the Automated Needle Wash

The automated needle wash can be programmed either as “injection with needle wash” or the needle wash can be included into the injector program. When the automated needle wash is used, the needle is moved into the wash port after the sample is drawn. By washing the needle after drawing a sample, the sample is removed from the outer surface of the needle immediately. As the flush port is automatically refilled with fresh wash solvent this option should be used routinely. Using wash vials is usually not necessary but available for special applications.

Using a wash vial

If a wash vial is used, it should be considered not to cap the vial. Otherwise small amounts of sample remain on the surface of the septum, which may be carried on the needle to the next sample.

Using the Flush Port

During the injection process when the sample is in the loop and when the valve still is in Bypass, the outside of the needle can be washed in a flush port located behind the injection port on the sampling unit. During the wash cycle as soon the needle is in the flush port a peristaltic pump fills the flush port with fresh solvent during a defined time. The volume of the flush port is about 680 μl and the pump delivers 6 ml/min. Setting the wash time to 10 seconds is sufficient to refill 2 times the flush port. In most cases this is enough to clean the needle outside. Additionally after the needle left the flush port the flush pump keeps running runs for 6 sec. to ensure refill with fresh solvent. At the end of this flush process – if “injection with needle wash” is selected – the needle returns to the injection port, the injection valve is switched to the mainpass position and directs the pump flow back through the sample loop.

For further information on how to reduce carry over see [“Optimization for Lowest Carry-Over”](#) on page 71

Recommended Wash Solvents

- water
- ethanol
- methanol
- water/acid (especially for basic compounds)
- water/base (especially for acidic compounds)
- water/acetonitrile

NOTE

The life time of the tubing in the peristaltic pump is shortened by the usage of organic solvents.

Cleaning the needle seat

If flush port has run out of solvent or the option “needle wash” hasn’t been used for several injections or in case the needle seat has got contaminated, the needle seat may be contaminated and carry-over is significantly higher than expected. For cleaning the needle seat there is an automatic procedure using the mobile phase’s solvents. If that doesn’t work a manual cleaning has to be done. the following procedure can be used to clean the needle seat

Automatic procedure

There’s an injector command for flushing the seat. So a cleaning method can be set up using an injector program.

Injector program

- INJECT
- FLUSH SEAT for 90.0 sec., 0.0 mm offset
- VALVE mainpass

Line 1 starts the run so the pump’s time table is started. Line 2 let’s the needle move above the seat and switches the valve to mainpass so that the pump’s solvent is directed through the loop and the needle onto the seat. The liquid leaves the seat via the drainage for the flush port. The offset can be used for getting a kind of blast pipe effect. Generally an offset of 0.0mm is a proper value. After the flush time (here 90sec) the valve is switched to bypass. Line 3 moves the needle back into the seat and switches valves back to main pass to restore hydraulic flow as it was before the cleaning process.

The pump's time table can be used if special solvents for cleaning are connected to the pump or if the flushing flow should be adjusted. Here's an illustrating example:

	Time	%B	Flow	Max. Press.
1	0.00	100.0		
2	0.10		0.500	
3	0.11		3.000	
4	0.70	100.0	3.000	
5	0.71	0.0	0.500	

Along with upper injector program this time table uses solvent B for cleaning the seat with an even higher flow rate than the perhaps limiting 0.5ml/min for column flow. To ensure that the flow rate isn't applied to the column and that column doesn't come in contact with flush solvent (in this case solvent B) choose a considerably long time (in this case 90sec) for flushing the seat in the injector program.

Manual procedure

If the automatic procedure doesn't succeed there is the semi-automatic seat back-flushing.

Preparation

- Move the needle to home position.
- Set pump flow to zero
- Connect the seat capillary with the pump capillary using a zero dead volume fitting.

Flushing

- Increase pump flow: The seat is flushed backwards, solvent bubbles over the seat and leaves the seat via the drainage for the flush port

Reconfigure system

- Set pump flow to zero
- Connect the pump outlet capillary to port 1 of injection valve
- Connect the seat capillary to port 5 of the injection valve.
- Reset the injector.

Fast Injection Cycle and Low Delay Volume

Short injection cycle times for high sample throughput is one of the main issues in analytical laboratories. Shortening cycle time starts with:

- shortening column length
- high flow rate
- steep gradient
- The detector balance may be set to OFF

General Recommendations for Fast Injection Cycle Times

As described in this section, the first step to provide short cycle times is optimizing the chromatographic conditions. Then the following Autosampler related issues should be considered:

- Use proper solvent for needle wash to decrease the wash time
- Reduce injection volume
- Increase eject speed
- Increase draw speed (if the viscosity of the sample and the solvent in Autosampler's flow path allows it)
- Do injection preparation in parallel with column equilibration (section "Overlapped Injection after gradient is flushed out")

Having optimized these parameters, further reduction of cycle times can be obtained if column equilibration is short compared to injector preparation or if automated column regeneration is configured. "Overlapped Injection during run mode" decreases this time between runs. But note that carry-over and discrimination may increase dramatically doing so.

Overlapped Injection After Gradient is Flushed Out

In this process the injection can be done in parallel to column equilibration phase without compromising any of the Autosampler's specifications.

This mode has one parameter. The time when to start the overlapped injection defined as "time after begin of run".

Considering a composition gradient that ends after 1 min. with reestablishing starting conditions the overlap time has to be set to somewhat above 1 min. to let the pump fill also the Autosampler's loop with start conditions.

Overlapped Injection During Run

In this process, as soon as the sample has reached the column, the injection valve is switched back to bypass and the next injection cycle is performed except for switching the injection valve to mainpass. This is done after actual run is finished and next analysis is started. Doing so the sample preparation time is saved as parallel to the run.

Switching the valve into the bypass position reduces the system delay volume by the complete Autosampler's flow path volume e.g. 270 ml for G1367B. Here the mobile phase is directed to the column without passing sample loop, needle and needle seat capillary. This can help to have faster cycle times especially if low flow rates have to be used like it is mandatory in narrow bore and micro bore HPLC.

NOTE

Having the valve in bypass position can increase the carry-over in the system.

The injection cycle times also depend on the injection volume. In identically standard condition, injecting 100 µl instead of 1 µl, increase the injection time by approximately 8 sec. In this case and if the viscosity of the sample allows it, the draw and eject speed of the injection system has to be increased.

Precise Injection Volume

Injection Volumes Less Than 2 μl

When the injection valve switches to the BYPASS position, the mobile phase in the sample loop is depressurized. When the syringe begins drawing sample, the mobile phase is further subjected to decreasing pressure. If the mobile phase is not adequately degassed, small gas bubbles may form in the sample loop during the injection sequence. When using injection volumes $< 2 \mu\text{l}$, these gas bubbles may affect the injection-volume precision. For best injection-volume precision with injection volumes $< 2 \mu\text{l}$, use of the Agilent 1200 Series degasser is recommended to ensure the mobile phase is adequately degassed. Also, using the automated needle wash between injections reduces carry-over to a minimum, improving injection-volume precision further.

Draw and Eject Speed

Draw Speed

The speed at which the metering unit draws sample out of the vial may have an influence on the injection volume precision when using viscous samples. If the draw speed is too high, air bubbles may form in the sample plug, affecting precision. The default draw speed is suitable for the majority of applications, however, when using viscous samples, set the draw speed to lower speed for optimum results. A “DRAW” statement in an injector program also uses the draw speed setting which is configured for the autosampler.

Eject Speed

The default draw speed is suitable for the majority of applications. When using large injection volumes, setting the eject speed to a higher value speeds up the injection cycle by shortening the time the metering unit requires to eject solvent at the beginning of the injection cycle (when the plunger returns to the home position).

An “EJECT” statement in an injector program also uses the eject speed setting which is configured for the autosampler. A faster eject speed shortens the time required to run the injector program. When using viscous samples, a high eject speed should be avoided.

Table 15 Draw and eject speed

	Draw speed (µl)	Eject speed (µl)
<i>High performance autosampler</i>		
Default value	200	200
Minimum	10	10
Maximum	1000	1000
<i>High performance autosampler SL+</i>		
Default value	100	100
Minimum	4	4
Maximum	1000	1000
<i>Micro Well Plate Autosampler with 8 µl loop capillary</i>		
Default value	4	10
Minimum	0.7	0.7
Maximum	20	100
<i>Micro Well Plate Autosampler with 40 µl loop capillary</i>		
Default value	4	10
Minimum	0.7	0.7
Maximum	250	250

Choice of Rotor Seal

Vespel™ Seal

The standard seal has sealing material made of Vespel. Vespel is suitable for applications using mobile phases within the pH range of 2.3 to 9.5, which is suitable for the majority of applications. However, for applications using mobile phases with pH below 2.3 or above 9.5, the Vespel seal may degrade faster, leading to reduced seal lifetime.

Tefzel™ Seal

For mobile phases with pH below 2.3 or above 9.5, or for conditions where the lifetime of the Vespel seal is drastically reduced, a seal made of Tefzel is available. Tefzel is more resistant than Vespel to extremes of pH, however, is a slightly *softer* material. Under normal conditions, the expected lifetime of the Tefzel seal is shorter than the Vespel seal, however, Tefzel may have the longer lifetime under more extreme mobile phase conditions.

PEEK Seal

With the High Performance SL+ Autosampler a PEEK rotor seal is used. This warrants a leak tight system at high pressures and allows the usage of solvents ranging from pH 2.3 to 12. The PEEK material may show a reduced lifetime if used with following solvents:

- Methylene chloride
- DMSO
- THF
- High concentrations of sulfuric acid
- High concentrations of nitric acid

Choice of Seat Capillary

The needle seat assembly is made up of two parts: needle seat and seat capillary.

Different models of seat capillaries are available.

p/n	Description
G1377-87101	Needle Seat (without capillary) for G1377A
G1375-87317	Seat Capillary (150 mm 0.10 mm ID) for G1377-87101 Needle Seat
G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat
G1375-87300	Seat Capillary (150 mm 0.05 mm ID) for G1377-87101 Needle Seat

Seat Capillary (150 mm 0.10 mm ID) for G1377-87101 Needle Seat (G1375-87317) is the capillary preinstalled in the micro well plate autosamplers upon delivery. This capillary is recommended for applications with a 0.3 mm column or higher. It provides less plugging of the capillary in general and especially with biological samples. For small K' this capillary can provide a higher peak width for isocratic analysis.

Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat (G1375-87316) is available as a spare part and is recommended for applications with a 0.3 mm column or smaller. This capillary gives full chromatographic performance.

Seat Capillary (150 mm 0.05 mm ID) for G1377-87101 Needle Seat (G1375-87300) is available as a spare part and is recommended for applications with a 0.3 mm column or smaller. This capillary gives full chromatographic performance. Due to the small diameter, this capillary can show some blockage.

5 **Optimizing Performance** Choice of Seat Capillary



6 Troubleshooting and Diagnostics

Overview of the Sampler's Indicators and Test Functions	86
Status Indicators	88
Power Supply Indicator	88
Module Status Indicator	89
Maintenance Functions	90
Sample Transport Self Alignment	91
Step Commands	92
Troubleshooting	93
Troubleshooting the Autosampler	94
Errors Which May Occur During the Turn ON and Initialization Process	95
Instrument Logbook Errors and Step by Step Repair Process	99
Needle Centering Over the Vial or the Well	104
Agilent Lab Advisor Software	105

This chapter gives an overview to troubleshooting the High Performance Micro Autosampler.



Overview of the Sampler's Indicators and Test Functions

Status Indicators

The autosampler is provided with two status indicators which indicate the operational state (prerun, not ready, run, and error states) of the instrument. The status indicators provide a quick visual check of the operation of the autosampler (see [“Status Indicators”](#) on page 88).

Error Messages

In the event of an electronic, mechanical or hydraulic failure, the instrument generates an error message in the user interface. For details on error messages and error handling, please refer to the Agilent Lab Monitor & Diagnostic Software.

Maintenance Functions

The maintenance functions position the needle assembly, the needle carrier, the sample transport assembly and the metering device for easy access when doing maintenance (see [“Maintenance Functions”](#) on page 90).

Sample Transport Self Alignment

The sample transport self alignment with the sampling unit and the well plate tray is required to compensate for larger deviations in positioning the needle carrier.

The sample transport self alignment is required after disassembling the system or when you exchange the sample transport, the sampling unit, the tray or the MTP main board.


This function is in the diagnose screen of the Chemstation or the Control Module.

Step Commands

The step functions enable execution of each step of the sampling sequence individually. The step functions are used primarily for troubleshooting, and for verification of correct autosampler operation after repair (see “[Step Commands](#)” on page 92). For details on step commands, please refer to the Agilent Lab Monitor & Diagnostic Software.

Status Indicators

Two status indicators are located on the front of the autosampler. The lower left indicates the power supply status, the upper right indicates the autosampler status.

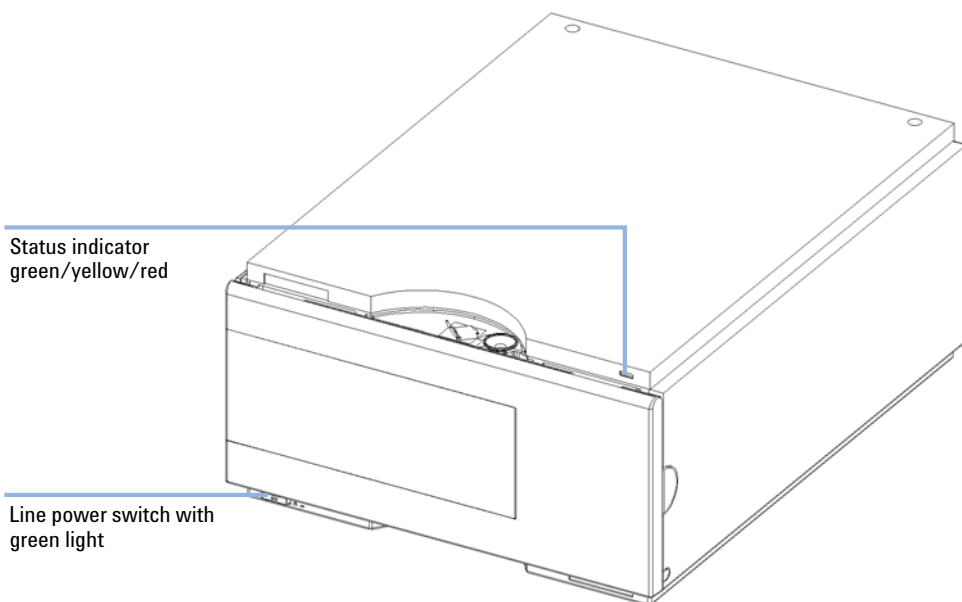

Power Supply Indicator

The power supply indicator is integrated into the main power switch. When the indicator is illuminated (*green*) the power is *ON*.

Module Status Indicator

The module status indicator indicates one of six possible module conditions:

- When the status indicator is *OFF* (and power switch light is on), the module is in a *prerun* condition, and is ready to begin an analysis.
- A *green* status indicator, indicates the module is performing an analysis (*run* mode).
- A *yellow* indicator indicates a *not-ready* condition. The module is in a not-ready state when it is waiting for a specific condition to be reached or completed (for example, immediately after changing a set point), or while a self-test procedure is running.
- An *error* condition is indicated when the status indicator is *red*. An error condition indicates the module has detected an internal problem which affects correct operation of the module. Usually, an error condition requires attention (e.g. leak, defective internal components). An error condition always interrupts the analysis.

If the error occurs during analysis, it is propagated within the LC system, i.e. a red LED may indicate a problem of a different module. Use the status display of your user interface for finding the root cause/module of the error.

- A *blinking* indicator indicates that the module is in resident mode (e.g. during update of main firmware).
- A *fast blinking* indicator indicates that the module is in a low-level error mode. In such a case try to re-boot the module or try a cold-start (see “[Special Settings](#)” on page 193. Then try a firmware update (see “[Replacing Module Firmware](#)” on page 154). If this does not help, a main board replacement is required.

Maintenance Functions

Some maintenance procedures require the needle arm, metering device, and needle carrier to be moved to specific positions to enable easy access to components. The maintenance functions move these assemblies into the appropriate maintenance position. In the ChemStation the sampler maintenance positions can be selected from the Maintenance menu in the Diagnosis display. In the Control Module the functions can be selected in the Test screens of the autosampler. In the Agilent Lab Monitor & Diagnostic Software the maintenance positions can be selected from the "Tools" icon.

Maintenance Functions

The maintenance functions moves the arm assembly in a specific position in order to enables easy access for maintenance operations

Home Position

The “home position” function moves the arm to the right side for better access and exchange of the trays

Park Position

The “park position” function moves the arm to the left side of the tray. In this position it is possible to secure the sample transport mechanism with the protection foam. The sample transport is than ready for transporting.

Change Piston

The “change-piston” function draws the piston away from the home position, relieving the tension on the spring. In this position, the analytical head assembly can be removed and reinstalled easily after maintenance. This position is also used to change the analytical head plunger and metering seal.

Table 16 Maintenance positions

Function	Arm position in X	Arm position in Theta	Arm Position in Z	Note
Change Needle	Left side	Straight	Up	No current on Theta
Change Carrier assembly	Left side	Straight	Middle	No current on the ST
Change Loop capillary	Middle	Left	Up	
Home position	Right side	Left rear	Up	
Park arm	Left side	Right rear	Up	

Sample Transport Self Alignment

The sample transport alignment with the sampling unit and the well plate tray is required to compensate for larger deviations in positioning the needle carrier. This function is in the diagnose screen of the Chemstation or the Control Module. In the Agilent Lab Monitor & Diagnostic Software, this function is in the "Calibration" icon.

The sample transport self alignment is required after disassembling the system or when you exchange:

- The sample transport.
- The sampling unit.
- The MTP main board.
- The autosampler tray base

Step Commands

Each movement of the sampling sequence can be done under manual control. This is useful during troubleshooting, where close observation of each of the sampling steps is required to confirm a specific failure mode or verify successful completion of a repair.

Each injector step command actually consists of a series of individual commands that move the autosampler components to predefined positions, enabling the specific step to be done.

Table 17 Step Commands

Step	Action	Comments
Valve Bypass	Switches injection valve to the bypass position.	
Plunger Home	Moves the plunger to the home position.	
Needle Up	Lifts the needle arm to the upper position.	Command also switches the valve to bypass if it is not already in that position.
Move to Location	Move the needle arm to the vial location on the plate.	
Needle into sample	Lowers the needle into the vial.	
Draw	Metering device draws the defined injection volume.	Command lifts the needle, and lowers the needle into sample. Command can be done more than once (maximum draw volume of 40/100/5000 µl cannot be exceeded). Use Plunger Home to reset the metering device.
Needle Up	Lifts the needle out of the vial.	
Needle into Seat	Lowers the needle arm into the seat.	
Valve Mainpass	Switches the injection valve to the mainpass position.	
Needle Up/Mainpass	Lifts the needle arm to the upper position and switches the injection valve to the mainpass position.	

Troubleshooting

If the autosampler is unable to perform a specific step due to a hardware failure, an error message is generated. You can use the step commands to perform an injection sequence, and observe how the autosampler responds to each command.

summarizes the step commands, and lists the error messages and probable causes associated with each possible failure.

Troubleshooting the Autosampler

Gather Information About the Problem

- When did the problem start?
- What was done/changed prior to the start of the problem?

In the Agilent Lab Monitor & Diagnostic Software the "Instrument Status Report" generates a report. This report includes the Instrument configuration with the instrument serial numbers and the firmware revisions, the instrument error history, the EMF editor, the result of the guided diagnostic and the method parameter (optional).

Errors Which May Occur During the Turn ON and Initialization Process

Failure to Turn ON

No activity when power button is pushed on. Power indicator stays off.

Probable cause

- 1 Defective main board.
- 2 Defective power supply.

Suggested actions

- Turn the sampler off. Disconnect the power supply from the main board, see if power indicator becomes green when the sampler is turned-on.
- If yes, change the main board (G1367-69520).
- Turn the sampler off. Disconnect the power supply from the main board, see if power indicator becomes green when the sampler is turned-on.
- If no, change the power supply (0905-2528 Rev G or higher).

Fan Failure

Early during the turn-on/initialization process a main fan or an exhaust fan error occurs.

Probable cause

- 1 Fan not connected to the main board
- 2 Fan connector defective
- 3 Defective fan.
- 4 Defective main board.

Suggested actions

- Make sure the fan is connected to the main board correctly
- Examine the fan connector for irregularities. Correct if possible
- Replace the defective fan (main fan: 3160-1017, exhaust fan: 3160-4097)
- Replace the main board (G1367-69520)

6 Troubleshooting and Diagnostics

Errors Which May Occur During the Turn ON and Initialization Process

Main Board Initialization Fails (I)

Status indicator remains off, but the rest of the turn-on/initialization process is successful.

Probable cause

- 1 The heel of the light pipe is not positioned correctly above the LED on the main board
- 2 Defective main board.

Suggested actions

- Correctly position the light pipe
- Replace the main board (G1367-69520)

Main Board Initialization Fails (II)

Status indicator remains off, and the rest of the turn-on/initialization process fails as well.

Probable cause

- 1

Suggested actions

- Refer to the possible causes and actions for step 5 below

Problem With the Vapor Blowout Period

The vapor blowout period does not end approximately 2 minutes after turn-on, initialization does not begin.

Probable cause

Suggested actions

- | | |
|---|--|
| <p>1 The front cover is not closed</p> | <p>Close the front cover. If the “front cover open” message is still displayed:</p> |
| <p>2 The front cover is closed, but the user interface displays a “front cover open” message</p> | <ul style="list-style-type: none"> • Make sure the front cover magnet is close enough to the magnet sensor • Check the ribbon cable from the SLS board to the main board • Replace the SLS board (G1367-66505) • replace the main board (G1367-69520) |
| <p>3 The left side cover is removed</p> | <p>Install the side door. If the “side door open” message is still displayed:</p> |
| <p>4 The left side cover is installed, but the user interface displays a “side cover open” message</p> | <ul style="list-style-type: none"> • Make sure the side cover magnet is present in the side door • Make sure the side cover magnet is oriented with the correct pole toward the magnet sensor on the main board and positioned in the side cover such that it is close enough to the magnet sensor • Replace the main board (G1367-69520) |

6 Troubleshooting and Diagnostics

Errors Which May Occur During the Turn ON and Initialization Process

Initialization Fails

The initialization fails to complete its required movements, resulting in one or more of a variety of possible error messages. The error message produced depends on when the failure occurred during the initialization.

Gather the revisions information, user interface error and logbook information, and error code information as described on page 1. Also, consider anything which may have been done just before the initialization failure occurred.

To date, we have seen initialization errors occur for a variety of reasons. As an overall troubleshooting plan, follow the suggested actions described below.

If this does not help, take the information from the instrument logbook, refer to the appropriate section in the next chapter and follow the recommended actions step by step.

Probable cause

1

Suggested actions

- Turn the sampler off, manually change the X-position of the sample transport and rotate the needle carrier to a different position, turn-on the sampler again.
- If there is any weight on top of the sampler, remove that weight, turn-off the sampler and then turn it on again.

Instrument Logbook Errors and Step by Step Repair Process

Instrument Logbook Errors and Step by Step Repair Process

The errors in the instrument logbook can be classified in 8 groups. In this section you can find a general step by step troubleshooting process for each of them.

1. Fan Error (Main Fan or Exhaust Fan)

Probable cause

1

Suggested actions

- Make sure the fan is connected to the main board correctly
- Examine the fan connector for irregularities. Correct if possible
- Replace the defective fan (main fan: 3160-1017, exhaust fan: 3160-4097)
- Replace the main board (G1367-69520)

2. Initialization Error

Probable cause

1

Suggested actions

- Upgrade the firmware revision to A.04.14 or higher and the ChemStation revision to A.08.04 or higher
- Check the sample transport connectors on the main board/sample transport
- Check the connector on the bottom of the sample transport unit
- Check for mechanical obstruction on the sample transport (X,Theta, Z)
- Change sample transport unit
- Change the main board (G1367-69520)

6 Troubleshooting and Diagnostics

Instrument Logbook Errors and Step by Step Repair Proces

3. Metering Sensor Error

Probable cause

1

Suggested actions

- Check the connectors on the SUD board
- Check the sampling unit connector on the main board
- Check the connector on the sampling unit
- Change the analytical head
- Change the sampling unit
- Change the main board (G1367-69520)

4. Rheodyne Valve Error

Probable cause

1

Suggested actions

- Turn the system off and on twice
- Check the connectors on the SUD board
- Check the sampling unit connector on the main board
- Check the connector on the sampling unit
- Change the rheodyne valve
- Change the sampling unit
- Change the main board (G1367-69520)

5. Needle Lock Error

Probable cause

1

Suggested actions

- Check the connectors on the SUD board
- Check the sampling unit connector on the main board
- Check the connector on the sampling unit
- Change the sampling unit
- Change the main board (G1367-69520)

6. Needle Into Seat Error

Probable cause

1

Suggested actions

- Upgrade the firmware revision to A.04.14 or higher and the ChemStation revision to A.08.04 or higher
- Check needle position and correct alignment in the pusher
- Perform an auto-alignment

6. Needle Into Seat Error (during initialization of the Sampler)

Probable cause

1

Suggested actions

- Turn-off the system
- Perform a forced cold start (move the 8-bit configuration dip switches 1,2,8 at the rear of the instrument to position 1)
- Turn-on the system
- Perform an auto-alignment
- Turn-off the system
- Move the 8-bit configuration dip switches 1,2,8 at the rear of the instrument to position 0
- Turn-on the system
- Check the connector from needle carrier to the sample transport unit
- Check the sample transport connectors on the main board/sample transport
- Check the connector on the bottom of the sample transport unit
- Change the needle carrier assembly (G1367-60010)
- Change the sample transport unit
- Change the main board (G1367-69520)

6 Troubleshooting and Diagnostics

Instrument Logbook Errors and Step by Step Repair Process

7. Needle / Seat Error

Probable cause

1

Suggested actions

- Upgrade the firmware revision to A.04.14 or higher and the ChemStation revision to A.08.04 or higher
- Check if the needle is installed (the sample transport comes without needle)
- Check the needle position and correct alignment in the pusher
- Check if the seat is not blocked with any parts or material (crystals, glass)
- Perform an auto-alignment
- Check the connector from the needle carrier to the sample transport unit
- Check the sample transport connectors on the main board/sample transport
- Check the connector on the bottom of the sample transport
- Change the needle and the seat
- Change the needle carrier assembly (G1367-60010)
- Change the sample transport unit
- Change the main board (G1367-69520)

8. Sample Location Error

Probable cause

1

Suggested actions

- Check the plate configuration in the user interface
- Ensure the right vials and plates are used
- Perform an auto-alignment
- Check the connector from the needle carrier to the sample transport unit
- Check the sample transport connectors on the main board/sample transport
- Check the connector on the bottom of the sample transport unit
- Change the needle and the seat
- Change the needle carrier assembly (G1367-60010)
- Change the sample transport unit
- Change the main board (G1367-69520)

Needle Centering Over the Vial or the Well

NOTE

The positioning of the needle is very precise. You have to take no action if the needle hits in the safe area.

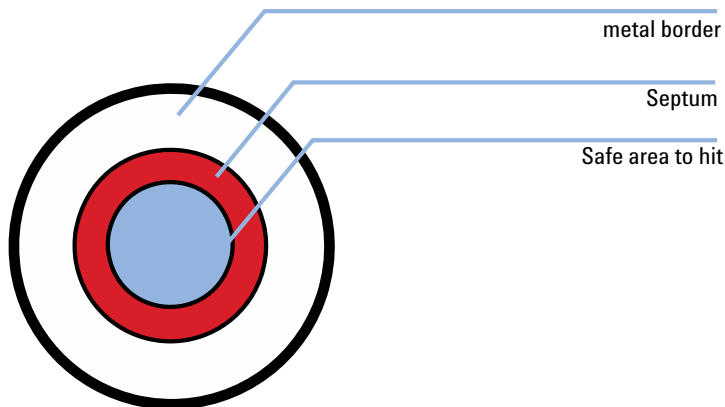


Figure 24 Vial cap

NOTE

If the diameter for the safe area is approximately *1 mm smaller* than the diameter of the septum, no corrective action is necessary.

Action to Take if the Needle Does Not Hit in the Safe Area

- ✓ Check if the right vials or plates are used (see “[List of Recommended Plates and Closing Mat](#)” on page 60 or “[List of Recommended Vials and Caps](#)” on page 62).
- ✓ Make sure that the needle is correctly installed. It should be pushed into the needle carrier as far forward as possible and centered in the vial pusher.
- ✓ Upgrade the firmware revision to A.04.14 or higher and the ChemStation revision to A.08.04 or higher.
- ✓ Perform an auto-alignment (without any plates in place).
- ✓ Change the tray G2258-60011 (see service note G1367-007).

Agilent Lab Advisor Software

The Agilent Lab Advisor software is a standalone product that can be used with or without data system. Agilent Lab Advisor software helps to manage the lab for high quality chromatographic results and can monitor in real time a single Agilent LC or all the Agilent GCs and LCs configured on the lab intranet.

Agilent Lab Advisor software provides diagnostic capabilities for all Agilent 1200 Infinity Series modules. This includes diagnostic capabilities, calibration procedures and maintenance routines for all the maintenance routines.

The Agilent Lab Advisor software also allows users to monitor the status of their LC instruments. The Early Maintenance Feedback (EMF) feature helps to carry out preventive maintenance. In addition, users can generate a status report for each individual LC instrument. The tests and diagnostic features as provided by the Agilent Lab Advisor software may differ from the descriptions in this manual. For details refer to the Agilent Lab Advisor software help files.

The Instrument Utilities is a basic version of the Lab Advisor with limited functionality required for installation, use and maintenance. No advanced repair, troubleshooting and monitoring functionality is included.

6 Troubleshooting and Diagnostics
Agilent Lab Advisor Software



7 Error Information

What Are Error Messages	109
General Error Messages	110
Timeout	110
Shutdown	111
Remote Timeout	111
Lost CAN Partner	112
Leak Sensor Short	112
Leak Sensor Open	113
Compensation Sensor Open	113
Compensation Sensor Short	114
Fan Failed	114
Leak	115
Open Cover	115
Module Specific Error Messages	116
Exhaust Fan Failed	116
Front Door Error	116
Side Door Error	117
Arm Movement Failed or Arm Movement Timeout	117
Valve to Bypass Failed	118
Valve to Mainpass Failed	118
Needle Lock Failed	119
Needle to Needle Seat Position	120
Needle Carrier Failed	121
Missing Vial or Missing Wash Vial	121
Initialization Failed	122
Metering Home Failed	123
Motor Temperature	124
Invalid Vial Position	125



7 Error Information

Agilent Lab Advisor Software

Peristaltic Pump Error	126
Vessel or Wash Vessel Error	126
Vessel Stuck to Needle	127

This chapter describes the meaning of error messages, and provides information on probable causes and suggested actions how to recover from error conditions.

What Are Error Messages

Error messages are displayed in the user interface when an electronic, mechanical, or hydraulic (flow path) failure occurs which requires attention before the analysis can be continued (for example, repair, or exchange of consumables is necessary). In the event of such a failure, the red status indicator at the front of the module is switched on, and an entry is written into the module logbook.

If an error occurs outside a method run, other modules will not be informed about this error. If it occurs within a method run, all connected modules will get a notification, all LEDs get red and the run will be stopped. Depending on the module type, this stop is implemented differently. For example, for a pump the flow will be stopped for safety reasons. For a detector, the lamp will stay on in order to avoid equilibration time. Depending on the error type, the next run can only be started, if the error has been resolved, for example liquid from a leak has been dried. Errors for presumably single time events can be recovered by switching on the system in the user interface.

Special handling is done in case of a leak. As a leak is a potential safety issue and may have occurred at a different module from where it has been observed, a leak always causes a shutdown of all modules, even outside a method run.

In all cases, error propagation is done via the CAN bus or via an APG remote cable (see documentation for the APG interface).

General Error Messages

General error messages are generic to all Agilent series HPLC modules and may show up on other modules as well.

Timeout

Error ID: 0062

The timeout threshold was exceeded.

Probable cause

- 1** The analysis was completed successfully, and the timeout function switched off the module as requested.
- 2** A not-ready condition was present during a sequence or multiple-injection run for a period longer than the timeout threshold.

Suggested actions

- Check the logbook for the occurrence and source of a not-ready condition. Restart the analysis where required.
- Check the logbook for the occurrence and source of a not-ready condition. Restart the analysis where required.

Shutdown

Error ID: 0063

An external instrument has generated a shutdown signal on the remote line.

The module continually monitors the remote input connectors for status signals. A LOW signal input on pin 4 of the remote connector generates the error message.

Probable cause	Suggested actions
1 Leak detected in another module with a CAN connection to the system.	Fix the leak in the external instrument before restarting the module.
2 Leak detected in an external instrument with a remote connection to the system.	Fix the leak in the external instrument before restarting the module.
3 Shut-down in an external instrument with a remote connection to the system.	Check external instruments for a shut-down condition.

Remote Timeout

Error ID: 0070

A not-ready condition is still present on the remote input. When an analysis is started, the system expects all not-ready conditions (for example, a not-ready condition during detector balance) to switch to run conditions within one minute of starting the analysis. If a not-ready condition is still present on the remote line after one minute the error message is generated.

Probable cause	Suggested actions
1 Not-ready condition in one of the instruments connected to the remote line.	Ensure the instrument showing the not-ready condition is installed correctly, and is set up correctly for analysis.
2 Defective remote cable.	Exchange the remote cable.
3 Defective components in the instrument showing the not-ready condition.	Check the instrument for defects (refer to the instrument's documentation).

Lost CAN Partner

Error ID: 0071

During an analysis, the internal synchronization or communication between one or more of the modules in the system has failed.

The system processors continually monitor the system configuration. If one or more of the modules is no longer recognized as being connected to the system, the error message is generated.

Probable cause

- 1 CAN cable disconnected.
- 2 Defective CAN cable.
- 3 Defective main board in another module.

Suggested actions

- Ensure all the CAN cables are connected correctly.
- Ensure all CAN cables are installed correctly.

Exchange the CAN cable.

Switch off the system. Restart the system, and determine which module or modules are not recognized by the system.

Leak Sensor Short

Error ID: 0082

The leak sensor in the module has failed (short circuit).

The current through the leak sensor is dependent on temperature. A leak is detected when solvent cools the leak sensor, causing the leak sensor current to change within defined limits. If the current increases above the upper limit, the error message is generated.

Probable cause

- 1 Defective leak sensor.
- 2 Leak sensor incorrectly routed, being pinched by a metal component.

Suggested actions

Please contact your Agilent service representative.

Please contact your Agilent service representative.

Leak Sensor Open

Error ID: 0083

The leak sensor in the module has failed (open circuit).

The current through the leak sensor is dependent on temperature. A leak is detected when solvent cools the leak sensor, causing the leak-sensor current to change within defined limits. If the current falls outside the lower limit, the error message is generated.

Probable cause	Suggested actions
<ol style="list-style-type: none"> 1 Leak sensor not connected to the main board. 	<p>Please contact your Agilent service representative.</p>
<ol style="list-style-type: none"> 2 Defective leak sensor. 	<p>Please contact your Agilent service representative.</p>
<ol style="list-style-type: none"> 3 Leak sensor incorrectly routed, being pinched by a metal component. 	<p>Please contact your Agilent service representative.</p>

Compensation Sensor Open

Error ID: 0081

The ambient-compensation sensor (NTC) on the main board in the module has failed (open circuit).

The resistance across the temperature compensation sensor (NTC) on the main board is dependent on ambient temperature. The change in resistance is used by the leak circuit to compensate for ambient temperature changes. If the resistance across the sensor increases above the upper limit, the error message is generated.

Probable cause	Suggested actions
<ol style="list-style-type: none"> 1 Defective main board. 	<p>Please contact your Agilent service representative.</p>

Compensation Sensor Short

Error ID: 0080

The ambient-compensation sensor (NTC) on the main board in the module has failed (open circuit).

The resistance across the temperature compensation sensor (NTC) on the main board is dependent on ambient temperature. The change in resistance is used by the leak circuit to compensate for ambient temperature changes. If the resistance across the sensor falls below the lower limit, the error message is generated.

Probable cause

- 1 Defective main board.

Suggested actions

Please contact your Agilent service representative.

Fan Failed

Error ID: 0068

The cooling fan in the module has failed.

The hall sensor on the fan shaft is used by the main board to monitor the fan speed. If the fan speed falls below a certain limit for a certain length of time, the error message is generated.

Depending on the module, assemblies (e.g. the lamp in the detector) are turned off to assure that the module does not overheat inside.

Probable cause

- 1 Fan cable disconnected.
- 2 Defective fan.
- 3 Defective main board.

Suggested actions

Please contact your Agilent service representative.

Please contact your Agilent service representative.

Please contact your Agilent service representative.

Leak

Error ID: 0064

A leak was detected in the module.

The signals from the two temperature sensors (leak sensor and board-mounted temperature-compensation sensor) are used by the leak algorithm to determine whether a leak is present. When a leak occurs, the leak sensor is cooled by the solvent. This changes the resistance of the leak sensor which is sensed by the leak-sensor circuit on the main board.

Probable cause

- 1 Loose fittings.
- 2 Broken capillary.

Suggested actions

- Ensure all fittings are tight.
- Exchange defective capillaries.

Open Cover

Error ID: 0205

The top foam has been removed.

Probable cause

- 1 Foam not activating the sensor.
- 2 Defective sensor or main board.

Suggested actions

Please contact your Agilent service representative.

Please contact your Agilent service representative.

Module Specific Error Messages

Exhaust Fan Failed

Error ID: 4456, 4457

The exhaust fan in the module has failed.

The hall sensor on the fan shaft is used by the main board to monitor the fan speed. If the fan speed falls below a certain value the error message is generated and the module shuts down.

Probable cause	Suggested actions
1 Fan cable disconnected.	Please contact your Agilent service representative.
2 Defective fan.	Please contact your Agilent service representative.
3 Defective main board.	Please contact your Agilent service representative.

Front Door Error

Error ID: 4350, 4352, 4458

The front door and/or the SLS board are damaged.

Probable cause	Suggested actions
1 The sensor on the SLS board is defective.	Please contact your Agilent service representative.
2 The door is bent or the magnet is misplaced/broken.	Please contact your Agilent service representative.

Side Door Error

Error ID: 4355, 4459

The side door and/or the main board are damaged.

Probable cause	Suggested actions
1 The door is bent or the magnet is misplaced/broken.	Please contact your Agilent service representative.
2 The sensor on the main board is defective.	Please contact your Agilent service representative.

Arm Movement Failed or Arm Movement Timeout

Error ID: 4002

The transport assembly was unable to complete a movement in one of the axes. The processor defines a certain time window for the successful completion of a movement in any particular axis. The movement and position of the transport assembly is monitored by the encoders on the stepper motors. If the processor does not receive the correct position information from the encoders within the time window, the error message is generated.

Axes identification:

- Arm Movement 0 Failed: X-axis.
- Arm Movement 1 Failed: Z-axis.
- Arm Movement 2 Failed: Theta (needle carrier rotation).

Probable cause	Suggested actions
1 Mechanical obstruction.	Ensure unobstructed movement of the transport assembly.
2 High friction in the transport assembly.	Please contact your Agilent service representative.
3 Defective motor assembly.	Please contact your Agilent service representative.
4 Defective sample transport assembly flex board.	Please contact your Agilent service representative.
5 Defective main board.	Please contact your Agilent service representative.

Valve to Bypass Failed

Error ID: 4014, 4701

The injection valve failed to switch to the bypass position.

The switching of the injection valve is monitored by two microswitches on the valve assembly. The switches detect the successful completion of the valve movement. If the valve fails to reach the bypass position, or if the microswitch does not close, the error message is generated.

Probable cause	Suggested actions
1 Valve in an intermediate position between the bypass and mainpass positions.	Turn the Autosampler main power OFF and ON.
2 Defective injection valve.	Please contact your Agilent service representative.
3 Defective main board.	Please contact your Agilent service representative.

Valve to Mainpass Failed

Error ID: 4015

The injection valve failed to switch to the mainpass position.

The switching of the injection valve is monitored by two microswitches on the valve assembly. The switches detect the successful completion of the valve movement. If the valve fails to reach the mainpass position, or if the microswitch does not close, the error message is generated.

Probable cause	Suggested actions
1 Valve in an intermediate position between the bypass and mainpass positions.	Turn the Autosampler main power OFF and ON.
2 Defective injection valve.	Please contact your Agilent service representative.
3 Defective main board.	Please contact your Agilent service representative.

Needle Lock Failed

Error ID: 4702, 4703

The lock assembly on the sampling unit failed to move successfully.

The upper and lower positions of the needle lock are monitored by position sensors on the sampling unit flex board. The sensors detect the successful completion of the needle lock movement. If the needle lock fails to reach the end point, or if the sensors fail to recognize the needle lock movement, the error message is generated.

Probable cause

- 1** Defective or dirty position sensor.
- 2** Sticking spindle assembly.
- 3** Defective needle drive motor
- 4** Defective main board.

Suggested actions

- Clean the position sensor.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

Needle to Needle Seat Position

Error ID: 4510, 4511, 4714

The needle failed to reach the end position in the needle seat.

The position of the needle is monitored by a position encoder on the needle carrier. If the needle fails to reach the end point, or if the encoder fails to recognize the needle carrier movement, the error message is generated.

Probable cause	Suggested actions
1 Bad sample transport/sampling unit alignment	Do an auto-alignment
2 Bent needle.	Check and exchange the needle assembly if necessary.
3 Missing needle.	Exchange the needle carrier assembly.
4 Blocked seat.	Clean or change the needle seat assembly if necessary.
5 Defective position sensor in the needle carrier assembly.	Please contact your Agilent service representative.
6 Defective main board.	Please contact your Agilent service representative.

Needle Carrier Failed

The needle carrier on the Sample Transport Assembly failed to move correctly.

Probable cause	Suggested actions
1 Defective Z-motor.	Please contact your Agilent service representative.
2 Vial pusher blocked.	Please contact your Agilent service representative.
3 Bad needle carrier positioning in X or Theta.	Please contact your Agilent service representative.
4 Defective vial pusher sensor.	Please contact your Agilent service representative.
5 Defective main board.	Please contact your Agilent service representative.

Missing Vial or Missing Wash Vial

Error ID: 4019, 4034, 4035, 4541, 4542, 4706, 4707

No vial was found in the position defined in the method or sequence.

When the needle carrier moves to a vial and the needle goes into the vial, the position of the needle is monitored by an encoder behind the vial pusher. If no vial is present, the encoder detects an error and the message “missing vial” is generated.

Probable cause	Suggested actions
1 No vial in the position defined in the method or sequence.	Install the sample vial in the correct position, or edit the method or sequence accordingly.
2 Defective needle carrier assembly.	Please contact your Agilent service representative.
3 Defective transport assembly flex board.	Please contact your Agilent service representative.
4 Defective main board.	Please contact your Agilent service representative.

Initialization Failed

Error ID: 4020

The autosampler failed to complete initialization correctly.

The autosampler initialization procedure moves the needle arm and transport assembly to their home positions in a predefined routine. During initialization, the processor monitors the position sensors and motor encoders to check for correct movement. If one or more of the movements is not successful, or is not detected, the error message is generated.

Probable cause	Suggested actions
1 Side door not installed correctly.	<ul style="list-style-type: none">• Check if the side door is installed correctly.• Check if the magnet is in place in the side door.
2 Sample transport/sampling unit not aligned correctly.	Do an auto-alignment
3 Mechanical obstruction.	Ensure unobstructed movement of the transport assembly.
4 Defective sampling unit flex board.	Please contact your Agilent service representative.
5 Defective transport assembly flex board.	Please contact your Agilent service representative.
6 Defective sampling unit motor.	Please contact your Agilent service representative.
7 Defective main board.	Please contact your Agilent service representative.

Metering Home Failed

Error ID: 4054, 4704

The metering piston has failed to move back to the home position.

The home position sensor on the sampling unit flex board monitors the home position of the piston. If the piston fails to move to the home position, or if the sensor fails to recognize the piston position, the error message is generated.

Probable cause

- 1** Dirty or defective sensor.
- 2** Broken plunger.
- 3** Defective metering-drive motor.
- 4** Defective main board.

Suggested actions

- Please contact your Agilent service representative.
- Exchange the metering plunger and seal.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

Motor Temperature

Error ID: 4027, 4040, 4261, 4451

One of the motors of the transport assembly has drawn excessive current, causing the motor to become too hot. The processor has switched off the motor to prevent damage to the motor.

Motor identification:

- Motor 0 temperature: X-axis motor.
- Motor 1 temperature: Z-axis motor.
- Motor 2 temperature: Theta motor.

The processor monitors the current drawn by each motor and the time the motor is drawing current. The current drawn by the motors is dependent on the load on each motor (friction, mass of components etc.). If the current drawn is too high, or the time the motor draws current is too long, the error message is generated.

Probable cause

- 1** Mechanical obstruction.
- 2** High friction in the transport assembly.
- 3** Motor belt tension too high.
- 4** Defective motor.
- 5** Defective transport assembly flex board.

Suggested actions

- Ensure unobstructed movement of the transport assembly.
- Please contact your Agilent service representative.
- Switch off the module at the power switch. Wait at least 10 minutes before switching on again.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

Invalid Vial Position

Error ID: 4042

The vial position defined in the method or sequence does not exist.

The reflection sensors on the transport assembly flex board are used to automatically check which sample trays are installed (coding on tray). If the vial position does not exist in the current sample tray configuration, the error message is generated.

Probable cause

- 1** Incorrect tray installed.
- 2** Incorrect tray definition.
- 3** Incorrect vial positions defined in the method or sequence.
- 4** Tray recognition defective (dirty sample tray or defective transport assembly flex board).

Suggested actions

- Install the correct trays, or edit the method or sequence accordingly.
- Install the correct trays, or edit the method or sequence accordingly.
- Install the correct trays, or edit the method or sequence accordingly.
- Ensure the coding surfaces of the sample tray are clean (located at the rear of the sample tray).
 - Please contact your Agilent service representative.

Peristaltic Pump Error

Error ID: 4514

The peristaltic pump motor in the autosampler has failed.

The current on the motor is used by the MTP board to monitor the speed of the peristaltic pump motor. If the current falls below a certain value, the error message is generated.

Probable cause

- 1 Defective motor.
- 2 Defective SUD board.
- 3 Defective main board.

Suggested actions

- Please contact your Agilent service representative.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

Vessel or Wash Vessel Error

Error ID: 4540, 4544, 4545, 4705, 4712

The needle does not reach the target position in the vial or in the vessel of the well plate.

The sensor behind the vial pusher in the needle carrier assembly detects the successful completion of the needle movement to the vessel. If the needle fails to reach the end point, the sensor fails to recognize the needle movement and the error message is generated.

Probable cause

- 1 Bad vessel definition in the plate configuration.
- 2 Closing mat too rigid/thick.
- 3 Bad X or Theta positioning.
- 4 Defective encoder on the needle carrier assembly.

Suggested actions

- Check the vessel definition in the plate configuration.
- Check that the closing mat is not too thick.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

Vessel Stuck to Needle

Error ID: 4453

The vessel sticks to the needle when the needle moves up.

Probable cause

- 1 Closing mat too rigid/thick.
- 2 Bad X or Theta positioning and the needle sticks into the wall between two holes.
- 3 Defective encoder on the needle carrier assembly.

Suggested actions

- Check that the closing mat is not too thick.
- Please contact your Agilent service representative.
- Please contact your Agilent service representative.

7 Error Information

Module Specific Error Messages



8 Maintenance

Introduction to Maintenance	130
Warnings and Cautions	131
Cleaning the Module	133
Maintenance Functions	134
Maintenance Procedures	135
Removing the Needle Assembly	136
Installing the Needle Assembly	138
Removing the Needle Carrier Assembly	140
Installing the Needle Carrier Assembly	141
Exchanging the Needle Seat	142
Exchanging the Seat Capillary	144
Exchanging the Rotor Seal	145
Metering Seal and Plunger	146
Removing the Metering Seal	146
Installing the Metering Seal	147
Removing the Loop Capillary	148
Installing the Loop Capillary	150
Replacing the Peristaltic Pump	152
Installing Interface Board	153
Replacing Module Firmware	154

This chapter describes the maintenance of the autosampler.



Introduction to Maintenance

The autosampler is designed for easy repair. The most frequent repairs such as changing a needle assembly can be done from the front of the instrument with the instrument in place in the system stack. These repairs are described in [“Maintenance Procedures”](#) on page 135.

Warnings and Cautions

WARNING

Toxic, flammable and hazardous solvents, samples and reagents

The handling of solvents, samples and reagents can hold health and safety risks.

- When working with these substances observe appropriate safety procedures (for example by wearing goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the vendor, and follow good laboratory practice.
 - The volume of substances should be reduced to the minimum required for the analysis.
 - Do not operate the instrument in an explosive atmosphere.
-

WARNING

Electrical shock

Repair work at the module can lead to personal injuries, e.g. shock hazard, when the cover is opened.

- Do not remove the cover of the module.
 - Only certified persons are authorized to carry out repairs inside the module.
-

WARNING

Personal injury or damage to the product

Agilent is not responsible for any damages caused, in whole or in part, by improper use of the products, unauthorized alterations, adjustments or modifications to the products, failure to comply with procedures in Agilent product user guides, or use of the products in violation of applicable laws, rules or regulations.

- Use your Agilent products only in the manner described in the Agilent product user guides.
-

8 Maintenance

Warnings and Cautions

CAUTION

Safety standards for external equipment

- If you connect external equipment to the instrument, make sure that you only use accessory units tested and approved according to the safety standards appropriate for the type of external equipment.
-

Cleaning the Module

To keep the module case clean, use a soft cloth slightly dampened with water, or a solution of water and mild detergent.

WARNING

Liquid dripping into the electronic compartment of your module can cause shock hazard and damage the module

- Do not use an excessively damp cloth during cleaning.
 - Drain all solvent lines before opening any connections in the flow path.
-

Maintenance Functions

Some maintenance procedures require the needle arm, metering device, and needle carrier to be moved to specific positions to enable easy access to components. The maintenance functions move these assemblies into the appropriate maintenance position. For details, refer to “[Maintenance Functions](#)” on page 90.

Maintenance Procedures

The procedures described in this section can be done with the autosampler in place in the stack. These procedures can be done on a more frequent basis.

Table 18 Simple Repair Procedures

Procedure	Typical Frequency	Notes
Exchanging the needle assembly	When the limit in the needle into seat counter in the EMF is exceeded. When needle shows indication of damage or blockage	See “Removing the Needle Assembly” on page 136
Exchanging the needle carrier assembly	When the needle carrier is defective	See “Removing the Needle Carrier Assembly” on page 140
Exchanging the needle seat assembly	When the limit in the needle into seat counter in the EMF is exceeded. When needle seat shows indication of damage or blockage	See “Exchanging the Needle Seat” on page 142
Exchanging the rotor seal	When the limit in the injector valve switches counter in the EMF is exceeded. When the valve performance shows indication of leakage or wear	See “Exchanging the Rotor Seal” on page 145
Exchanging the metering seal	When autosampler reproducibility indicates seal wear	See “Removing the Metering Seal” on page 146
Exchanging the loop capillary	When loop capillary blocked or broken	See “Removing the Loop Capillary” on page 148
Exchanging the peristaltic pump	When tubing broken	See “Replacing the Peristaltic Pump” on page 152

Removing the Needle Assembly

- When**
- When the needle is visibly damaged
 - When the needle is blocked

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)

Parts required	#	p/n	Description
	1	G1377-87201	Needle assembly

WARNING

Risk of injury by uncovered needle

An uncovered needle is a risk of harm to the operator.

- Be careful working at the needle carrier assembly.
- Use the silicon safety tube supplied with every new needle.

- 1 In the user interface start the maintenance mode and select the “Change Needle/Seat” function. In the Agilent Lab Monitor & Diagnostic Software the “Change Needle/Seat” function can be found in the “Tools” icon.
- 2 Open the front door and remove the side door.
- 3 Remove the plate tray from the tray base.
- 4 Push the silicon safety tube, supplied in the WPS leak kit (G1367-60006) and with every new needle, over the needle.
- 5 Unlock the needle tighter lock system.
- 6 Loosen the loop capillary fitting on the analytical head side.
- 7 Remove the loop capillary corrugated waste tube.
- 8 Pinch the holder clamp, pull back and remove the needle assembly with the loop capillary from the needle carrier.

- 9 Attach the 5/16 inch wrench to hold position at the needle assembly.
Use the 4 mm wrench to loosen the fitting of the loop capillary.

NOTE

Do not bend the sheet metal of the needle.

- 10 Pull the loop capillary out from the needle assembly.

Installing the Needle Assembly

- When**
- When the needle is visibly damaged
 - When the needle is blocked

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)

Parts required	#	p/n	Description
	1	G1377-87201	Needle assembly

WARNING

Risk of injury by uncovered needle

An uncovered needle is a risk of harm to the operator.

- Be careful working at the needle carrier assembly.
- Use the silicon safety tube supplied with every new needle.

- 1 Push the silicon safety tube, supplied in the WPS leak kit (G1367-60006) and with every new needle, over the needle.
- 2 Pull the loop capillary in the new needle assembly (G1367-87201, G1367-87202 or G1377-87201).
- 3 Attach the 5/16 inch wrench to hold position at the needle assembly. Use the 4 mm wrench to tighten the fitting of the loop capillary.

NOTE

Do not hold the needle during this step to avoid bending it.

- 4 Push the loop capillary into the loop capillary protection tube until it comes out on the sampling unit side.
- 5 Tighten the loop capillary fitting to the analytical head.
- 6 Install the loop capillary corrugated waste tube over the loop capillary.

- 7 Pinch the holder clamp and reinsert the needle assembly into the needle carrier.
- 8 Lock the needle tighter lock system.
- 9 Push the black chain into the needle assy until the stop.
- 10 Check the alignment of the needle in the needle pusher of the needle carrier by viewing from several directions to see that it is aligned in the center of the needle pusher.

NOTE

The needle must be centered in the needle pusher as all alignment by the autosampler is calculated from the needle pusher position.

- 11 Remove the silicon safety tube from the needle.
- 12 Replace the plate tray in the tray base. Re-install the side door and close the front door.
- 13 In the user interface close the "Change Needle/Seat" function and exit the maintenance mode. In the Agilent Lab Monitor & Diagnostic Software the "Change Needle/Seat" function can be found in the "Tools" icon.

Removing the Needle Carrier Assembly

When When the needle carrier is defect

Tools required	p/n	Description
	8710-2438	Hexagonal key, 2 mm

Parts required	#	p/n	Description
	1	G1367-60010	Needle Carrier assembly

WARNING

Risk of injury by uncovered needle

An uncovered needle is a risk of harm to the operator.

- Be careful working at the needle carrier assembly.
- Use the silicon safety tube supplied with every new needle.

- 1 In the user interface start the maintenance mode and select the "Change Needle Carrier" function. In the Agilent Lab Monitor & Diagnostic Software the "Change Needle Carrier" function can be found in the "Tools" icon.
- 2 Open the front door and remove the side door.
- 3 Remove the plate tray from the tray base.
- 4 Push the silicon safety tube, supplied in the WPS leak kit (G1367-60006) and with every new needle, over the needle.
- 5 Pinch the holder clamp, pull back and remove the needle assembly from the needle carrier.
- 6 Unplug the flex board on the sample transport.
- 7 Unscrew the three holding hex screws with the 2 mm hex key.
- 8 Remove the needle carrier assy.

Installing the Needle Carrier Assembly

When When the needle carrier is defect

Tools required	p/n	Description
	8710-2438	Hexagonal key, 2 mm

Parts required	#	p/n	Description
	1	G1367-60010	Needle Carrier assembly

- 1 Install a new needle carrier (G1367-60010) on place
- 2 Install the three holding hex screws with the 2 mm hex key.
- 3 Plug in the flex board on the sample transport.
- 4 Push the silicon safety tube, supplied in the WPS leak kit (G1367-60006) and with every new needle, over the needle.
- 5 Pinch the holder clamp and reinsert the needle assembly into the needle carrier.
- 6 Check the alignment of the needle in the needle pusher of the needle carrier by viewing from several directions to see that it is aligned in the center of the needle pusher.

NOTE

The needle must be centered in the needle pusher as all alignment by the autosampler is calculated from the needle pusher position.

- 7 Remove the silicon safety tube from the needle.
- 8 Replace the plate tray in the tray base.
- 9 Re-install the side door and close the front door.
- 10 In the user interface close the "Change Needle Carrier" function and exit the maintenance mode. The instrument will reset. In the Agilent Lab Monitor & Diagnostic Software the "Change Needle Carrier" function can be found in the "Tools" icon.

Exchanging the Needle Seat

- When**
- When the seat is visibly damaged
 - When the seat capillary is blocked

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)
		Screwdriver, flat

Parts required	#	p/n	Description
	1	G1377-87101	Needle Seat (without capillary) for G1377A
	1	G1375-87317	Seat Capillary (150 mm 0.10 mm ID) for G1377-87101 Needle Seat
	1	G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat
	1	G1375-87300	Seat Capillary (150 mm 0.05 mm ID) for G1377-87101 Needle Seat

- 1** In the user interface start the maintenance mode and select the "Change Needle/Seat" function. In the Agilent Lab Monitor & Diagnostic Software the "change needle/seat" function can be found under the "Tools" icon.
- 2** Open the front door and remove the side door.
- 3** Remove the plate tray from the tray base.
- 4** Disconnect the seat capillary from the needle seat with the 4 mm open wrench.
- 5** Use the flat-head screwdriver to remove the needle seat.
- 6** Insert the new needle seat. Press it firmly in position.
- 7** Connect the seat capillary to the needle seat with the 4 mm open wrench.
- 8** Replace the plate tray in the tray base. Re-install the side door and close the front door.

- 9 In the user interface close the “Change Needle/Seat” function and exit the maintenance mode. In the Agilent Lab Monitor & Diagnostic Software the "change needle/seat" function can be found under the "Tools" icon.

NOTE

The seat capillary can be exchanged alone if the needle seat is not damaged.

Exchanging the Seat Capillary

- When**
- When the seat is visibly damaged
 - When the seat capillary is blocked

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)
		Screwdriver, flat

Parts required	#	p/n	Description
	1	G1375-87317	Seat Capillary (150 mm 0.10 mm ID) for G1377-87101 Needle Seat
	1	G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat
	1	G1375-87300	Seat Capillary (150 mm 0.05 mm ID) for G1377-87101 Needle Seat
	1	G1377-87101	Needle Seat (without capillary) for G1377A

- 1** Disconnect the seat capillary from the injection valve (port 5) with the 1/4 - 5/16 inch wrench.
- 2** Remove the needle seat, see [“Exchanging the Needle Seat”](#) on page 142.
- 3** Use the seat capillary mounting tool (provided in the accessory kit) and replace the seat capillary from the seat with the 4 mm wrench.
- 4** Install the seat assembly in its location and reconnect the capillary to the injection valve (port 5).
- 5** Follow the procedure in [“Exchanging the Needle Seat”](#) on page 142 to finish the installation.

NOTE

Choose the seat capillary diameter, as function of the column and the application you run on the system. See, [“Choice of Seat Capillary”](#) on page 83.

Exchanging the Rotor Seal

- When**
- When poor injection-volume reproducibility
 - When leaking injection valve

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-2394	Hex key 9/64 inch 15 cm long T-handle

Parts required	#	p/n	Description
	1	0100-2088	Vespel Rotor Seal for 0101-1050 injection valve (G1377A)

- 1** Open the front door.
- 2** Remove all capillaries from the injection-valve ports with the 1/4 inch wrench.
- 3** Unscrew and remove the three stator screws from the stator head with the 9/64 inch wrench.
- 4** Remove the stator head, the stator face and the stator ring.
- 5** Remove the rotor seal (and isolation seal if required).
- 6** Install the new rotor seal and isolation seal (if required). The metal spring inside the isolation seal must face toward the valve body. In other words, the metal spring should not be visible when the isolation seal is installed.
- 7** Reinstall the stator ring.
- 8** Place the stator face on the stator head. The pins on the stator face must engage in the holes on the stator head.
- 9** Install this stator head/face assy on the injection valve. Tighten the screws alternately with the 9/64 inch wrench until the stator head is secure.
- 10** Reconnect all the capillaries to the injection valve ports with the 1/4 inch wrench.
- 11** Close the front cover.

Metering Seal and Plunger

Removing the Metering Seal

- When**
- When poor injection-volume reproducibility
 - When leaking metering device

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)
	8710-2392	Hexagonal key, 4 mm, 15 cm long, T-handle (supplied in accessory kit)
		Screwdriver, small flat head

Parts required	Description
	None

- 1** In the user interface start the maintenance mode and select the "Change Piston" function. In the Agilent Lab Monitor & Diagnostic Software the "Change Piston" function can be found under the "Tools" icon.
- 2** Open the front door
- 3** Remove the corrugated leak tubing
- 4** Remove the two capillaries from the analytical head (Use a 1/4 inch wrench if you have a SST capillary or a 4 mm wrench if you have a fused silica capillary).
- 5** Unscrew alternately the two fixing screws with the 4 mm hex key and remove them.
- 6** Pull the analytical head away from the sampling unit.
- 7** Remove the two fixing screws from the base of the analytical head.
- 8** Remove the head body.
- 9** Using the piston, carefully remove the metering seal. Clean the chamber and ensure all particular matter is removed.

Installing the Metering Seal

- When**
- When poor injection-volume reproducibility
 - When leaking metering device

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open
	8710-1534	Wrench, 4 mm open end (supplied in accessory kit)
	8710-2392	Hexagonal key, 4 mm, 15 cm long, T-handle (supplied in accessory kit)
		Screwdriver, small flat head

Parts required	#	p/n	Description
	1	5022-2175	Metering Seal (pack of 1) for the G1377-60013 40 µL Analytical Head
OR	1	0905-1717	Metering seal for smallest leak rates
	1	5064-8293	Micro Plunger assembly

- 1** Install the new metering seal. Press it firmly into position.
- 2** Reassemble the analytical head. Press the plunger assembly into the seal.
- 3** Put the two fixing screws in place and reinstall the analytical head to the sampling unit.
- 4** Tighten alternately the two fixing screws with the 4 mm hex key.
- 5** Connect the two capillaries to the analytical head (Use a 1/4 inch wrench if you have a SST capillary or a 4 mm wrench if you have a fused silica capillary).
- 6** Reinstall the corrugated leak tubing.
- 7** Close the front door.
- 8** In the user interface close the “Change Piston” function and exit the maintenance mode. In the Agilent Lab Monitor & Diagnostic Software the "Change Piston" function can be found under the "Tools" icon.

Removing the Loop Capillary

- When**
- Capillary blocked
 - Capillary broken

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open

Parts required	#	p/n	Description
	1	G1375-87315	Loop capillary (injection volume up to 8 µL)
	1	G1377-87300	Loop capillary, 40 µL for G1377A

WARNING

Risk of injury by uncovered needle

An uncovered needle is a risk of harm to the operator.

- Be careful when you remove the loop capillary.
- Use the silicon safety tube for the needle.

NOTE

If the loop capillary is not broken and no solvent has leaked into the loop capillary tube, the solvent draw up steps using the syringe can be skipped (steps 5, 6, 8).

- 1 In the user interface start the maintenance mode and select the "Change Loop Capillary" function. In the Agilent Lab Monitor & Diagnostic Software the "Change Loop Capillary" function can be found under the "Tools" icon.
- 2 Open the front door and remove the side door.
- 3 Remove the plate tray from the tray base.
- 4 Push the silicon safety tube over the needle
- 5 Remove the corrugated loop capillary waste tube and introduce the small tubing from the leak kit into the loop capillary protection tube.
- 6 Draw up the liquid with the syringe.

- 7 Unlock the needle tighter lock system.
- 8 Draw up the rest of the solvent from the loop capillary protection tube.
- 9 Loosen the loop capillary fitting on the analytical head side.
- 10 Pinch the holder clamp, pull back and remove the needle assembly with the loop capillary from the needle carrier.
- 11 Attach the 5/16 inch wrench to hold position at the needle assembly.
Use the 4 mm wrench to loosen the fitting of the loop capillary.
- 12 Pull the loop capillary out from the needle assembly.

Installing the Loop Capillary

When Capillary blocked
Capillary broken

Tools required	p/n	Description
	8710-0510	Wrench, 1/4 - 5/16 inch, open

Parts required	#	p/n	Description
	1	G1375-87315	Loop capillary (injection volume up to 8 µL)
	1	G1377-87300	Loop capillary, 40 µL for G1377A

- 1 Pull the new loop capillary in the needle assembly.
- 2 Attach the 5/16 inch wrench to hold position at the needle assembly. Use the second wrench to tighten the loop capillary fitting.
- 3 Push the loop capillary into the loop capillary protection tube until it comes out on the sampling unit side.
- 4 Re install the loop capillary corrugated waste tube over the loop capillary.
- 5 Retighten the loop capillary fitting on the analytical head.
- 6 Pinch the holder clamp and reinsert the needle assembly into the needle carrier.
- 7 Push the black chain into the needle assembly until the stop.
- 8 Lock the needle tighter lock system.
- 9 Check the alignment of the needle in the needle pusher of the needle carrier by viewing from several directions to see that it is aligned in the center of the needle pusher.

NOTE

The needle must be centered in the needle pusher as all alignment by the autosampler is calculated from the needle pusher position.

- 10 Remove the silicon safety tube from the needle.

- 11 Replace the plate tray in the tray base. Re-install the side door and close the front door.
- 12 In the user interface close the "Change Loop Capillary" function and exit the maintenance mode. In the Agilent Lab Monitor & Diagnostic Software the "Change Loop Capillary" function can be found under the "Tools" icon.

Replacing the Peristaltic Pump

When • Tubing blocked or broken.

Tools required **Description**
Sand paper

Parts required	#	p/n	Description
	1	5065-4445	Peristaltic pump with Pharmed tubing

NOTE

The peristaltic pump is a replaceable unit. The tubing inside the pump is not replaceable.

- 1 Remove the corrugated leak tubing.
- 2 Press the two clips on the front of the peristaltic pump.
- 3 Pull the pump forward off the motor shaft.
- 4 Disconnect the tubing leading to the wash port and the tubing coming from the solvent bottle.
- 5 Connect the wash port tubing to the upper tubing of the new pump (use sandpaper to get a good grip on the tubing).
- 6 Connect the tubing coming from the solvent bottle to the lower tubing of the new pump.
- 7 Push the pump onto the motor shaft until the clips click into place.
- 8 Reinstall the corrugated leak tubing.

Installing Interface Board

When • For all repairs inside the sampler or for installation of the board.

Tools required Flat head screwdriver

Parts required	#	Description
	1	Interface board

CAUTION

Electrostatic discharge at the interface board

The interface board is sensitive to electrostatic discharge.

→ Always use the ESD strap when handling electronic boards.

- 1 Switch off the autosampler at the main power switch.
- 2 Disconnect all cables from the existing interface board. Then loosen the interface board holding screws and slide the board out of its holding rails.
- 3 Identify the interface board slot cover. Loosen the two holding screws, and remove the cover.
- 4 Carefully insert the new interface board into the holding rails, and push the board into the slot. Make sure the board plugs into the socket correctly.
- 5 Reconnect all cables to the new interface board.
- 6 Switch on the sampler.
- 7 Configuring optional Interface board, see “BCD / External Contact Board” on page 194 and “LAN Communication Interface Board” on page 196.

Replacing Module Firmware

When	The installation of newer firmware might be necessary <ul style="list-style-type: none">• if a newer version solves problems of older versions or• to keep all systems on the same (validated) revision. The installation of older firmware might be necessary <ul style="list-style-type: none">• to keep all systems on the same (validated) revision or• if a new module with newer firmware is added to a system or• if third party control software requires a special version.
-------------	---

Tools required	Description
	LAN/RS-232 Firmware Update Tool
OR	Agilent Lab Advisor software
OR	Instant Pilot G4208A (only if supported by module)

Parts required	#	Description
	1	Firmware, tools and documentation from Agilent web site

Preparations Read update documentation provided with the Firmware Update Tool.

To upgrade/downgrade the module's firmware carry out the following steps:

- 1 Download the required module firmware, the latest LAN/RS-232 FW Update Tool and the documentation from the Agilent web.
 - http://www.chem.agilent.com/_layouts/agilent/downloadFirmware.aspx?whid=69761
- 2 For loading the firmware into the module follow the instructions in the documentation.

Module Specific Information

There is no specific information for this module.



9 Parts for Maintenance

Sampler Main Assemblies 156

Vial Trays 158

Accessory Kits 160

Thermostat for ALS/FC/Spotter 161

This chapter provides information on parts for maintenance.



Sampler Main Assemblies

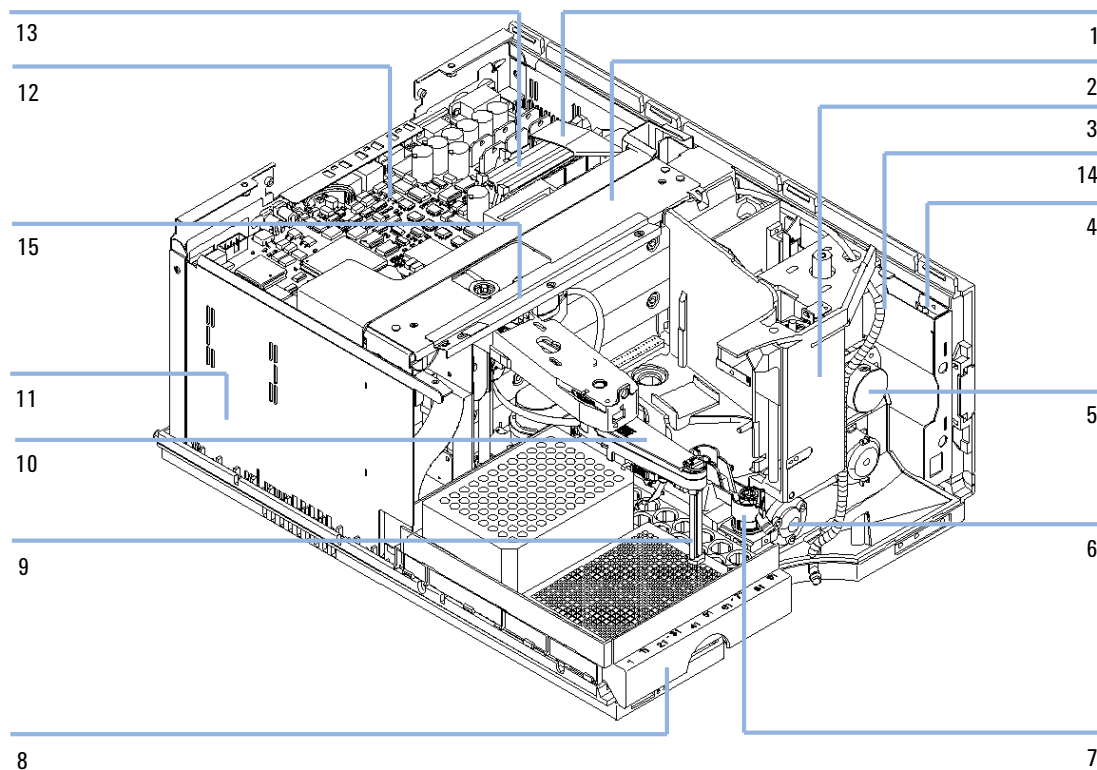


Figure 25 Autosampler Main Assemblies

Item	p/n	Description
1	G1313-81602	Ribbon Cable (from SU to MTB)
2	G1377-60009	Sample transport assembly
	G1377-69009	Sample transport assembly (refurbished exchange part)
3	G1367-60028	Sampling unit
	G1377-60008	Sampling unit (assy comes without injection valve and analytical head)
4	G1367-66505	SLS board (not shown)

Item	p/n	Description
5	G1377-60013	Analytical Head Assembly (40 µL)
6	0101-1050	Micro injection valve assembly
7	G1377-87000	Needle Seat Assembly for G1377A (0.10 mm ID)
	G1377-87001	Needle Seat Assembly for G1377A (0.075 mm ID)
	G1377-87002	Needle Seat Assembly for G1377A (0.05 mm ID)
7	G1377-87101	Needle Seat (without capillary) for G1377A (Legacy part)
	G1375-87317	Seat Capillary (150 mm 0.10 mm ID) for G1377-87101 Needle Seat (Legacy part)
	G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat (Legacy part)
	G1375-87300	Seat Capillary (150 mm 0.05 mm ID) for G1377-87101 Needle Seat (Legacy part)
8	G2258-60011	Standard tray for two well plates + 10 x 2 ml vials
9	G1377-87201	Needle assembly
10	G1367-60010	Needle Carrier assembly
11	0950-5274	Power supply (not visible)
12	G1367-66520	MTP main board
	G1367-69520	Exchange MTP main board
13	G1364-81601	Ribbon cable (from ST to MTP)
	G1367-81600	Ribbon cable (from SLS to MTP) (not visible)
14	G1375-87315	Loop capillary (injection volume up to 8 µL)
	G1377-87300	Loop capillary, 40 µL for G1377A
15	G1367-60040	Illumination assembly
	G1375-87304	Fused silica/PEEK capillary 50 µm, 50 cm from sampler to TCC
	3160-1017	Fan (not visible)
	3160-4097	Exhaust fan (not visible)
	G1351-68701	Interface board (BCD) with external contacts and BCD outputs (not visible)

Vial Trays

Table 19 Autosampler Vial Trays and Tray Base

Item	Description	Part Number
1	Tray for 2 plates + 10 × 2-ml vials	p/n G2258-60011
2	Screws for springs	p/n 0515-0866
3	Spring	p/n G1313-09101
4	Spring stud	p/n 0570-1574
5	Tray base (includes items 4,5,6)	p/n G1329-60000
6	Adapter air channel	p/n G1329-43200
	Plug channel (not shown)	p/n G1367-47200

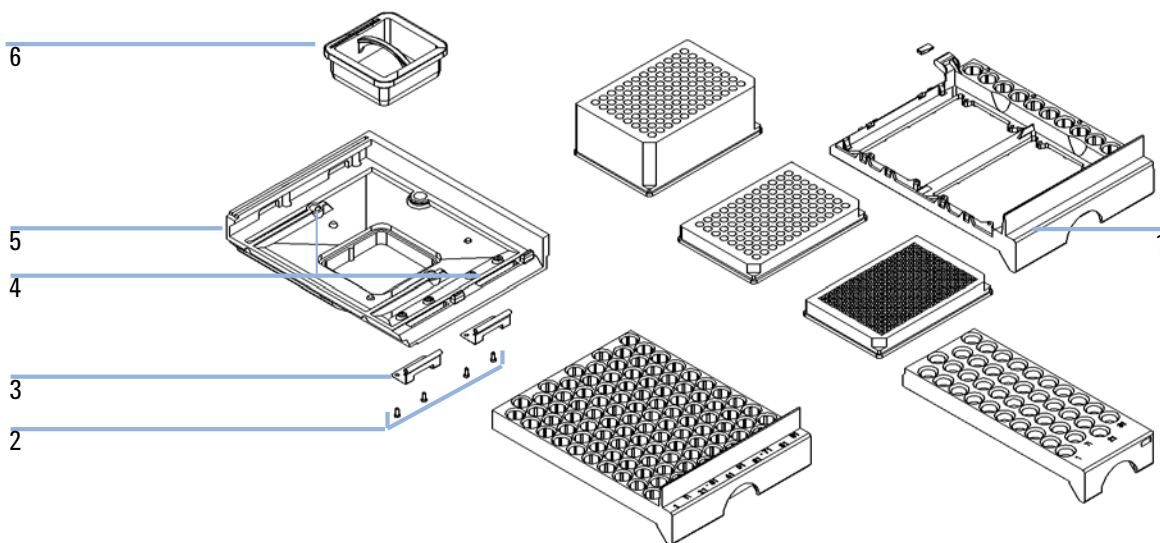


Figure 26 Vial trays and Tray Base

Table 20 Recommended plates and closing mat

Description	Rows	Columns	Plate height	Volume (µl)	Part Number	Package
384Agilent	16	24	14.4	80	p/n 5042-1388	30
384Corning	16	24	14.4	80	No Agilent PN	
384Nunc	16	24	14.4	80	No Agilent PN	
96Agilent	8	12	14.3	400	p/n 5042-1386 p/n 5042-1385	10 120
96Agilent conical	8	12	17.3	150	p/n 5042-8502	25
96CappedAgilent	8	12	47.1	300	p/n 5065-4402	1
96Corning	8	12	14.3	300	No Agilent PN	
96CorningV	8	12	14.3	300	No Agilent PN	
96DeepAgilent31mm	8	12	31.5	1000	p/n 5042-6454	50
96DeepNunc31mm	8	12	31.5	1000	No Agilent PN	
96DeepRitter41mm	8	12	41.2	800	No Agilent PN	
96Greiner	8	12	14.3	300	No Agilent PN	
96GreinerV	8	12	14.3	250	No Agilent PN	
96Nunc	8	12	14.3	400	No Agilent PN	
Closing mat for all 96 Agilent plates	8	12			p/n 5042-1389	50

Table 21 Recommended Vial plates

Description	Part Number
Vial plate for 54x2ml vials (6/pk)	p/n G2255-68700
Vial plate for 15x6ml vials (1/pk)	p/n 5022-6539
Vial plate for 27 Eppendorf tubes (1/pk)	p/n 5022-6538

Accessory Kits

p/n	Description
5063-6527	Tubing assembly, i.d. 6 mm, o.d. 9 mm, 1.2 m (to waste)
9222-0518	Bag - plastics
G1315-45003	Torque adapter
G1367-60006	WPS Leak Kit
G1375-87304	Fused silica/PEEK capillary 50 μ m, 50 cm
G1375-87316	Seat Capillary (150 mm 0.075 mm ID) for G1377-87101 Needle Seat
G1329-43200	Adapter air channel
5181-1519	CAN cable, Agilent module to module, 1 m
8710-1534	Wrench, 4 mm both ends, open end
G1377-44900	tool for Micro Seat Capillary Mounting
G1377-87300	Loop capillary, 40 μ L for G1377A

Thermostat for ALS/FC/Spotter

Table 22 Thermostat for ALC/FC/Spotter

Item	Description	Part Number
1	Thermostat, exchange assembly	p/n G1330-69040

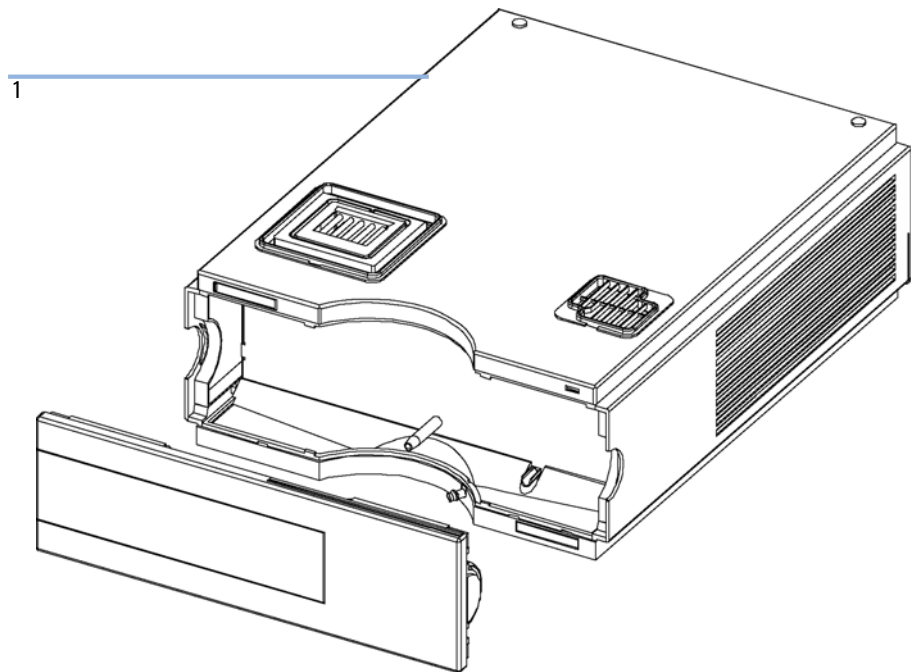


Figure 27 Thermostat for ALS/FC/Spotter

9 **Parts for Maintenance**
Thermostat for ALS/FC/Spotter



10 Identifying Cables

Cable Overview	164
Analog Cables	166
Remote Cables	168
BCD Cables	171
CAN/LAN Cables	173
External Contact Cable	174
RS-232 Cables	175
Agilent 1200 Module to Printer	176

This chapter provides information on cables used with the Agilent 1200 Infinity Series modules.



Cable Overview

NOTE

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.

Analog cables

p/n	Description
35900-60750	Agilent module to 3394/6 integrators
35900-60750	Agilent 35900A A/D converter
01046-60105	Analog cable (BNC to general purpose, spade lugs)

Remote cables

p/n	Description
03394-60600	Agilent module to 3396A Series I integrators 3396 Series II / 3395A integrator, see details in section “Remote Cables” on page 168
03396-61010	Agilent module to 3396 Series III / 3395B integrators
5061-3378	Remote Cable
01046-60201	Agilent module to general purpose

BCD cables

p/n	Description
03396-60560	Agilent module to 3396 integrators
G1351-81600	Agilent module to general purpose

CAN cables

p/n	Description
5181-1516	CAN cable, Agilent module to module, 0.5 m
5181-1519	CAN cable, Agilent module to module, 1 m

LAN cables

p/n	Description
5023-0203	Cross-over network cable, shielded, 3 m (for point to point connection)
5023-0202	Twisted pair network cable, shielded, 7 m (for point to point connection)


External Contact Cable

p/n	Description
G1103-61611	External contact cable - Agilent module interface board to general purposes

RS-232 cables


p/n	Description
G1530-60600	RS-232 cable, 2 m
RS232-61601	RS-232 cable, 2.5 m Instrument to PC, 9-to-9 pin (female). This cable has special pin-out, and is not compatible with connecting printers and plotters. It's also called "Null Modem Cable" with full handshaking where the wiring is made between pins 1-1, 2-3, 3-2, 4-6, 5-5, 6-4, 7-8, 8-7, 9-9.
5181-1561	RS-232 cable, 8 m

Analog Cables




One end of these cables provides a BNC connector to be connected to Agilent modules. The other end depends on the instrument to which connection is being made.


Agilent Module to 3394/6 Integrators

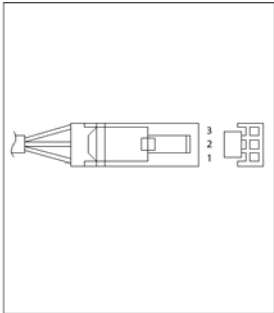p/n 35900-60750	Pin 3394/6	Pin Agilent module	Signal Name
	1		Not connected
	2	Shield	Analog -
	3	Center	Analog +

Agilent Module to BNC Connector

p/n 8120-1840	Pin BNC	Pin Agilent module	Signal Name
	Shield	Shield	Analog -
	Center	Center	Analog +

Agilent Module to General Purpose

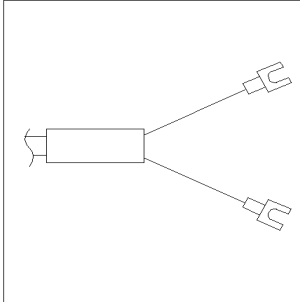p/n 01046-60105	Pin	Pin Agilent module	Signal Name
	1		Not connected
	2	Black	Analog -
	3	Red	Analog +

Remote Cables



One end of these cables provides a Agilent Technologies APG (Analytical Products Group) remote connector to be connected to Agilent modules. The other end depends on the instrument to be connected to.


Agilent Module to 3396A Integrators

p/n 03394-60600	Pin 3396A	Pin Agilent module	Signal Name	Active (TTL)
<p>A diagram of the Agilent module connector, a vertical rectangular component with a latch on the right side. It has 15 pins. Pins 1, 3, 5, 7, 9, 13, and 15 are labeled with their respective numbers.</p>	9	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	3	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	5,14	7 - Red	Ready	High
	1	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low
	13, 15		Not connected	


Agilent Module to 3396 Series II / 3395A Integrators

Use the cable Agilent module to 3396A Series I integrators (03394-60600) and cut pin #5 on the integrator side. Otherwise the integrator prints START; not ready.

Agilent Module to 3396 Series III / 3395B Integrators

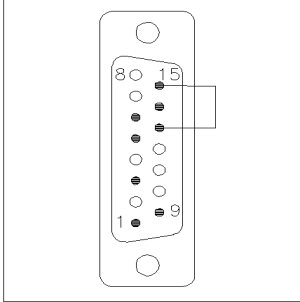p/n 03396-61010	Pin 33XX	Pin Agilent module	Signal Name	Active (TTL)
	9	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	3	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	14	7 - Red	Ready	High
	4	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low
	13, 15		Not connected	


Agilent Module to Agilent 35900 A/D Converters

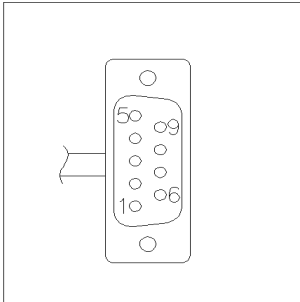p/n 5061-3378	Pin 35900 A/D	Pin Agilent module	Signal Name	Active (TTL)
	1 - White	1 - White	Digital ground	
	2 - Brown	2 - Brown	Prepare run	Low
	3 - Gray	3 - Gray	Start	Low
	4 - Blue	4 - Blue	Shut down	Low
	5 - Pink	5 - Pink	Not connected	
	6 - Yellow	6 - Yellow	Power on	High
	7 - Red	7 - Red	Ready	High
	8 - Green	8 - Green	Stop	Low
	9 - Black	9 - Black	Start request	Low

10 Identifying Cables

Remote Cables

Agilent Module to General Purpose

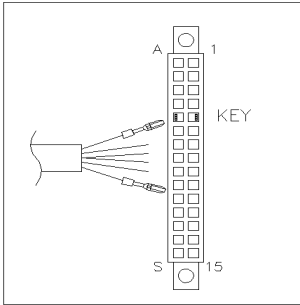p/n 01046-60201	Wire Color	Pin Agilent module	Signal Name	Active (TTL)
	White	1	Digital ground	
	Brown	2	Prepare run	Low
	Gray	3	Start	Low
	Blue	4	Shut down	Low
	Pink	5	Not connected	
	Yellow	6	Power on	High
	Red	7	Ready	High
	Green	8	Stop	Low
	Black	9	Start request	Low

BCD Cables



One end of these cables provides a 15-pin BCD connector to be connected to the Agilent modules. The other end depends on the instrument to be connected to


Agilent Module to General Purpose

p/n G1351-81600	Wire Color	Pin Agilent module	Signal Name	BCD Digit
	Green	1	BCD 5	20
	Violet	2	BCD 7	80
	Blue	3	BCD 6	40
	Yellow	4	BCD 4	10
	Black	5	BCD 0	1
	Orange	6	BCD 3	8
	Red	7	BCD 2	4
	Brown	8	BCD 1	2
	Gray	9	Digital ground	Gray
	Gray/pink	10	BCD 11	800
	Red/blue	11	BCD 10	400
	White/green	12	BCD 9	200
	Brown/green	13	BCD 8	100
	not connected	14		
	not connected	15	+ 5 V	Low


10 Identifying Cables

BCD Cables

Agilent Module to 3396 Integrators

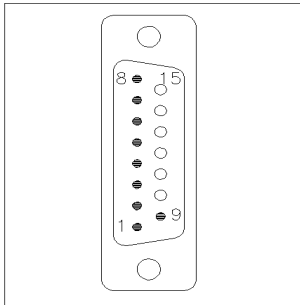p/n 03396-60560	Pin 3396	Pin Agilent module	Signal Name	BCD Digit
	1	1	BCD 5	20
	2	2	BCD 7	80
	3	3	BCD 6	40
	4	4	BCD 4	10
	5	5	BCD0	1
	6	6	BCD 3	8
	7	7	BCD 2	4
	8	8	BCD 1	2
	9	9	Digital ground	
	NC	15	+ 5 V	Low

CAN/LAN Cables



Both ends of this cable provide a modular plug to be connected to Agilent modules CAN or LAN connectors.


CAN Cables

p/n	Description
5181-1516	CAN cable, Agilent module to module, 0.5 m
5181-1519	CAN cable, Agilent module to module, 1 m

LAN Cables

p/n	Description
5023-0203	Cross-over network cable, shielded, 3 m (for point to point connection)
5023-0202	Twisted pair network cable, shielded, 7 m (for point to point connection)

External Contact Cable



One end of this cable provides a 15-pin plug to be connected to Agilent modules interface board. The other end is for general purpose.

Agilent Module Interface Board to general purposes

p/n G1103-61611	Color	Pin Agilent module	Signal Name
	White	1	EXT 1
	Brown	2	EXT 1
	Green	3	EXT 2
	Yellow	4	EXT 2
	Grey	5	EXT 3
	Pink	6	EXT 3
	Blue	7	EXT 4
	Red	8	EXT 4
	Black	9	Not connected
	Violet	10	Not connected
	Grey/pink	11	Not connected
	Red/blue	12	Not connected
	White/green	13	Not connected
	Brown/green	14	Not connected
	White/yellow	15	Not connected

RS-232 Cables

p/n	Description
G1530-60600	RS-232 cable, 2 m
RS232-61601	RS-232 cable, 2.5 m Instrument to PC, 9-to-9 pin (female). This cable has special pin-out, and is not compatible with connecting printers and plotters. It's also called "Null Modem Cable" with full handshaking where the wiring is made between pins 1-1, 2-3, 3-2, 4-6, 5-5, 6-4, 7-8, 8-7, 9-9.
5181-1561	RS-232 cable, 8 m

10 Identifying Cables

Agilent 1200 Module to Printer

Agilent 1200 Module to Printer

p/n	Description
5181-1529	Cable Printer Serial & Parallel, is a SUB-D 9 pin female vs. Centronics connector on the other end (NOT FOR FW UPDATE). For use with G1323 Control Module.



11 Hardware Information

Firmware Description	178
Electrical Connections	181
Rear View of the Module	182
Interfaces	183
Overview Interfaces	186
Setting the 8-bit Configuration Switch (without On-board) LAN	190
Communication Settings for RS-232C	191
Special Settings	193
Optional Interface Boards	194
Instrument Layout	198
Early Maintenance Feedback	199

This chapter describes the module in more detail on hardware and electronics.



Firmware Description

The firmware of the instrument consists of two independent sections:

- a non-instrument specific section, called *resident system*
- an instrument specific section, called *main system*

Resident System

This resident section of the firmware is identical for all Agilent 1100/1200/1220/1260/1290 series modules. Its properties are:

- the complete communication capabilities (CAN, LAN and RS-232C)
- memory management
- ability to update the firmware of the 'main system'

Main System

Its properties are:

- the complete communication capabilities (CAN, LAN and RS-232C)
- memory management
- ability to update the firmware of the 'resident system'

In addition the main system comprises the instrument functions that are divided into common functions like

- run synchronization through APG remote,
- error handling,
- diagnostic functions,
- or module specific functions like
 - internal events such as lamp control, filter movements,
 - raw data collection and conversion to absorbance.

Firmware Updates

Firmware updates can be done using your user interface:

- PC and Firmware Update Tool with local files on the hard disk
- Instant Pilot (G4208A) with files from a USB Flash Disk
- Agilent Lab Advisor software B.01.03 and above

The file naming conventions are:

PPPP_RVVV_XXX.dlb, where

PPPP is the product number, for example, 1315AB for the G1315A/B DAD,

R the firmware revision, for example, A for G1315B or B for the G1315C DAD,

VVV is the revision number, for example 102 is revision 1.02,

XXX is the build number of the firmware.

For instructions on firmware updates refer to section *Replacing Firmware* in chapter "Maintenance" or use the documentation provided with the *Firmware Update Tools*.

NOTE

Update of main system can be done in the resident system only. Update of the resident system can be done in the main system only.

Main and resident firmware must be from the same set.

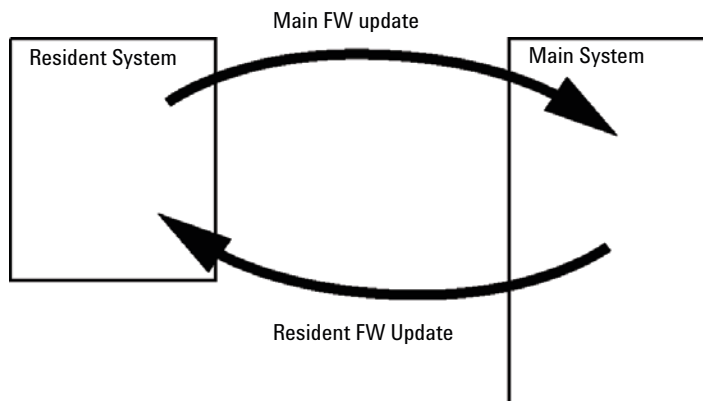


Figure 28 Firmware Update Mechanism

NOTE

Some modules are limited in downgrading due to their main board version or their initial firmware revision. For example, a G1315C DAD SL cannot be downgraded below firmware revision B.01.02 or to a A.xx.xx.

Some modules can be re-branded (e.g. G1314C to G1314B) to allow operation in specific control software environments. In this case the feature set of the target type are use and the feature set of the original are lost. After re-branding (e.g. from G1314B to G1314C), the original feature set is available again.

All these specific informations are described in the documentation provided with the firmware update tools.

The firmware update tools, firmware and documentation are available from the Agilent web.

- http://www.chem.agilent.com/_layouts/agilent/downloadFirmware.aspx?whid=69761

Electrical Connections

- The CAN bus is a serial bus with high speed data transfer. The two connectors for the CAN bus are used for internal module data transfer and synchronization.
- One analog output provides signals for integrators or data handling systems.
- The interface board slot is used for external contacts and BCD bottle number output or LAN connections.
- The REMOTE connector may be used in combination with other analytical instruments from Agilent Technologies if you want to use features such as start, stop, common shut down, prepare, and so on.
- With the appropriate software, the RS-232C connector may be used to control the module from a computer through a RS-232C connection. This connector is activated and can be configured with the configuration switch.
- The power input socket accepts a line voltage of 100 – 240 VAC \pm 10 % with a line frequency of 50 or 60 Hz. Maximum power consumption varies by module. There is no voltage selector on your module because the power supply has wide-ranging capability. There are no externally accessible fuses, because automatic electronic fuses are implemented in the power supply.

NOTE

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.

Rear View of the Module

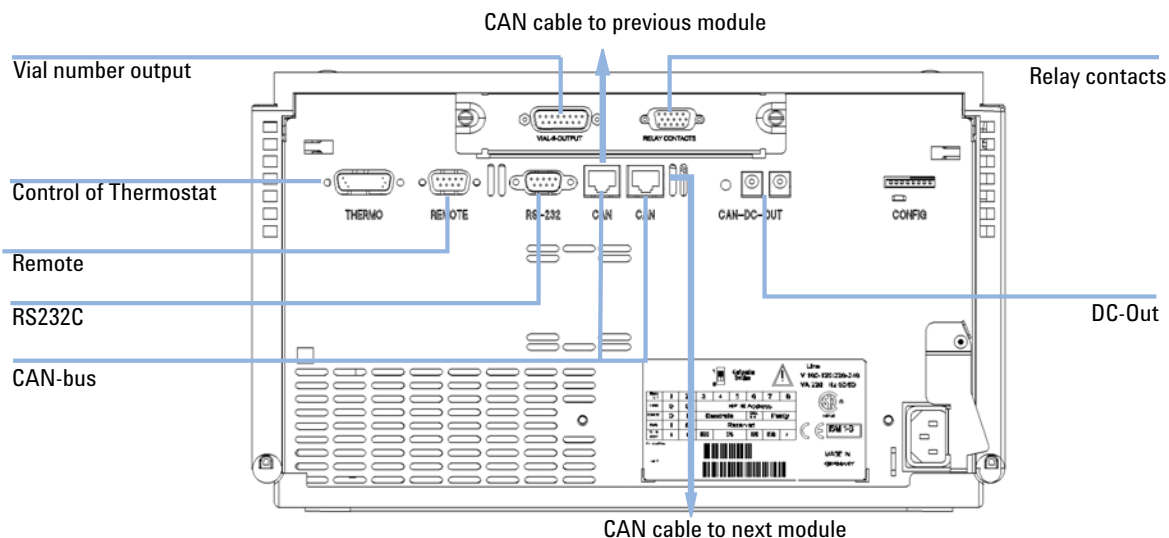


Figure 29 Autosampler Electrical Connections

Interfaces

The Agilent 1200 Infinity Series modules provide the following interfaces:

Table 23 Agilent 1200 Infinity Series Interfaces

Module	CAN	LAN/BCD (optional)	LAN (on-board)	RS-232	Analog	APG Remote	Special
Pumps							
G1310B Iso Pump G1311B Quat Pump G1311C Quat Pump VL G1312B Bin Pump K1312B Bin Pump Clinical Ed. G1312C Bin Pump VL 1376A Cap Pump G2226A Nano Pump G5611A Bio-inert Quat Pump	2	Yes	No	Yes	1	Yes	
G4220A/B Bin Pump G4204A Quat Pump	2	No	Yes	Yes	No	Yes	CAN-DC- OUT for CAN slaves
G1361A Prep Pump	2	Yes	No	Yes	No	Yes	CAN-DC- OUT for CAN slaves
Samplers							
G1329B ALS G2260A Prep ALS	2	Yes	No	Yes	No	Yes	THERMOSTAT for G1330B/K1330B
G1364B FC-PS G1364C FC-AS G1364D FC- μ S G1367E HiP ALS K1367E HiP ALS Clinical Ed. G1377A HiP micro ALS G2258A DL ALS G5664A Bio-inert FC-AS G5667A Bio-inert Autosampler	2	Yes	No	Yes	No	Yes	THERMOSTAT for G1330B/K1330B CAN-DC- OUT for CAN slaves
G4226A ALS	2	Yes	No	Yes	No	Yes	

11 Hardware Information

Interfaces

Table 23 Agilent 1200 Infinity Series Interfaces

Module	CAN	LAN/BCD (optional)	LAN (on-board)	RS-232	Analog	APG Remote	Special
Detectors							
G1314B VWD VL G1314C VWD VL+	2	Yes	No	Yes	1	Yes	
G1314E/F VWD K1314F Clinical Ed.	2	No	Yes	Yes	1	Yes	
G4212A/B DAD K4212B DAD Clinical Ed.	2	No	Yes	Yes	1	Yes	
G1315C DAD VL+ G1365C MWD G1315D DAD VL G1365D MWD VL	2	No	Yes	Yes	2	Yes	
G1321B FLD K1321B FLD Clinical Ed. G1321C FLD	2	Yes	No	Yes	2	Yes	
G1362A RID	2	Yes	No	Yes	1	Yes	
G4280A ELSD	No	No	No	Yes	Yes	Yes	EXT Contact AUTOZERO
Others							
G1170A Valve Drive	2	No	No	No	No	No	1
G1316A/C TCC K1316C TCC Clinical Ed.	2	No	No	Yes	No	Yes	
G1322A DEG K1322A DEG Clinical Ed.	No	No	No	No	No	Yes	AUX
G1379B DEG	No	No	No	Yes	No	Yes	
G4225A DEG K4225A DEG Clinical Ed.	No	No	No	Yes	No	Yes	

Table 23 Agilent 1200 Infinity Series Interfaces

Module	CAN	LAN/BCD (optional)	LAN (on-board)	RS-232	Analog	APG Remote	Special
G4227A Flex Cube	2	No	No	No	No	No	CAN-DC- OUT for CAN slaves 1
G4240A CHIP CUBE	2	Yes	No	Yes	No	Yes	CAN-DC- OUT for CAN slaves THERMOSTAT for G1330A/B (NOT USED), K1330B

¹ Requires a HOST module with on-board LAN (e.g. G4212A or G4220A with minimum firmware B.06.40 or C.06.40) or with additional G1369C LAN Card

NOTE

The detector (DAD/MWD/FLD/VWD/RID) is the preferred access point for control via LAN. The inter-module communication is done via CAN.

- CAN connectors as interface to other modules
- LAN connector as interface to the control software
- RS-232C as interface to a computer
- REMOTE connector as interface to other Agilent products
- Analog output connector(s) for signal output

Overview Interfaces

CAN

The CAN is inter-module communication interface. It is a 2-wire serial bus system supporting high speed data communication and real-time requirement.

LAN

The modules have either an interface slot for an LAN card (e.g. Agilent G1369B/C LAN Interface) or they have an on-board LAN interface (e.g. detectors G1315C/D DAD and G1365C/D MWD). This interface allows the control of the module/system via a PC with the appropriate control software. Some modules have neither on-board LAN nor an interface slot for a LAN card (e.g. G1170A Valve Drive or G4227A Flex Cube). These are hosted modules and require a Host module with firmware B.06.40 or later or with additional G1369C LAN Card.

NOTE

If an Agilent detector (DAD/MWD/FLD/VWD/RID) is in the system, the LAN should be connected to the DAD/MWD/FLD/VWD/RID (due to higher data load). If no Agilent detector is part of the system, the LAN interface should be installed in the pump or autosampler.

RS-232C (Serial)

The RS-232C connector is used to control the module from a computer through RS-232C connection, using the appropriate software. This connector can be configured with the configuration switch module at the rear of the module. Refer to *Communication Settings for RS-232C*.

NOTE

There is no configuration possible on main boards with on-board LAN. These are pre-configured for

- 19200 baud,
- 8 data bit with no parity and
- one start bit and one stop bit are always used (not selectable).

The RS-232C is designed as DCE (data communication equipment) with a 9-pin male SUB-D type connector. The pins are defined as:

Table 24 RS-232C Connection Table

Pin	Direction	Function
1	In	DCD
2	In	RxD
3	Out	TxD
4	Out	DTR
5		Ground
6	In	DSR
7	Out	RTS
8	In	CTS
9	In	RI

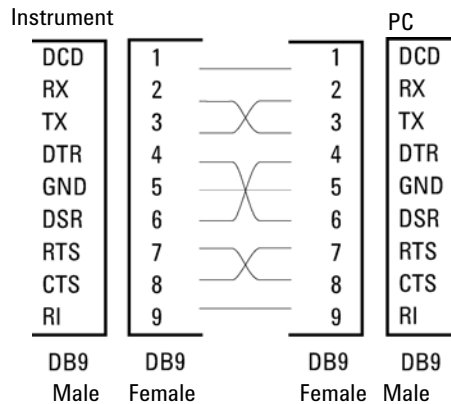


Figure 30 RS-232 Cable

Analog Signal Output

The analog signal output can be distributed to a recording device. For details refer to the description of the module's main board.

APG Remote

The APG Remote connector may be used in combination with other analytical instruments from Agilent Technologies if you want to use features as common shut down, prepare, and so on.

Remote control allows easy connection between single instruments or systems to ensure coordinated analysis with simple coupling requirements.

The subminiature D connector is used. The module provides one remote connector which is inputs/outputs (wired- or technique).

To provide maximum safety within a distributed analysis system, one line is dedicated to **SHUT DOWN** the system's critical parts in case any module detects a serious problem. To detect whether all participating modules are switched on or properly powered, one line is defined to summarize the **POWER ON** state of all connected modules. Control of analysis is maintained by signal readiness **READY** for next analysis, followed by **START** of run and optional **STOP** of run triggered on the respective lines. In addition **PREPARE** and **START REQUEST** may be issued. The signal levels are defined as:

- standard TTL levels (0 V is logic true, + 5.0 V is false),
- fan-out is 10 ,
- input load is 2.2 kOhm against + 5.0 V, and
- output are open collector type, inputs/outputs (wired- or technique).

NOTE

All common TTL circuits operate with a 5 V power supply. A TTL signal is defined as "low" or L when between 0 V and 0.8 V and "high" or H when between 2.0 V and 5.0 V (with respect to the ground terminal).

Table 25 Remote Signal Distribution

Pin	Signal	Description
1	DGND	Digital ground
2	PREPARE	(L) Request to prepare for analysis (for example, calibration, detector lamp on). Receiver is any module performing pre-analysis activities.
3	START	(L) Request to start run / timetable. Receiver is any module performing run-time controlled activities.
4	SHUT DOWN	(L) System has serious problem (for example, leak: stops pump). Receiver is any module capable to reduce safety risk.
5		Not used
6	POWER ON	(H) All modules connected to system are switched on. Receiver is any module relying on operation of others.
7	READY	(H) System is ready for next analysis. Receiver is any sequence controller.
8	STOP	(L) Request to reach system ready state as soon as possible (for example, stop run, abort or finish and stop injection). Receiver is any module performing run-time controlled activities.
9	START REQUEST	(L) Request to start injection cycle (for example, by start key on any module). Receiver is the autosampler.

Special Interfaces

There is no special interface for this module.

Setting the 8-bit Configuration Switch (without On-board) LAN

The 8-bit configuration switch is located at the rear of the module.

This module does not have its own on-board LAN interface. It can be controlled through the LAN interface of another module, and a CAN connection to that module.

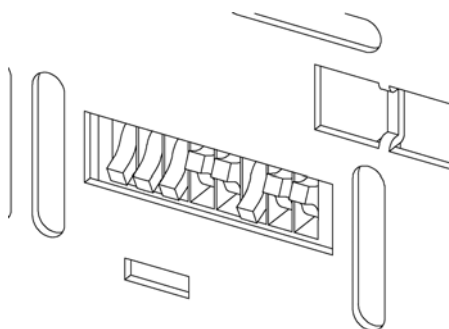


Figure 31 Configuration switch (settings depend on configured mode)

All modules without on-board LAN:

- default should be ALL DIPS DOWN (= best settings)
 - Bootp mode for LAN and
 - 19200 baud, 8 data bit / 1 stop bit with no parity for RS-232
- DIP 1 DOWN and DIP 2 UP allows special RS-232 settings
- for boot/test modes DIPS 1+2 must be UP plus required mode

NOTE

For normal operation use the default (best) settings.

Switch settings provide configuration parameters for serial communication protocol and instrument specific initialization procedures.

NOTE

With the introduction of the Agilent 1260 Infinity, all GPIB interfaces have been removed. The preferred communication is LAN.

NOTE

The following tables represent the configuration switch settings for the modules without on-board LAN only.

Table 26 8-bit Configuration Switch (without on-board LAN)

Mode Select	1	2	3	4	5	6	7	8
RS-232C	0	1	Baudrate			Data Bits	Parity	
Reserved	1	0	Reserved					
TEST/BOOT	1	1	RSVD	SYS		RSVD	RSVD	FC

NOTE

The LAN settings are done on the LAN Interface Card G1369B/C. Refer to the documentation provided with the card.

Communication Settings for RS-232C

The communication protocol used in the column compartment supports only hardware handshake (CTS/RTR).

Switches 1 in down and 2 in up position define that the RS-232C parameters will be changed. Once the change has been completed, the column instrument must be powered up again in order to store the values in the non-volatile memory.

Table 27 Communication Settings for RS-232C Communication (without on-board LAN)

Mode Select	1	2	3	4	5	6	7	8
RS-232C	0	1	Baudrate			Data Bits	Parity	

Use the following tables for selecting the setting which you want to use for RS-232C communication. The number 0 means that the switch is down and 1 means that the switch is up.

11 Hardware Information

Setting the 8-bit Configuration Switch (without On-board) LAN

Table 28 Baudrate Settings (without on-board LAN)

Switches			Baud Rate	Switches			Baud Rate
3	4	5		3	4	5	
0	0	0	9600	1	0	0	9600
0	0	1	1200	1	0	1	14400
0	1	0	2400	1	1	0	19200
0	1	1	4800	1	1	1	38400

Table 29 Data Bit Settings (without on-board LAN)

Switch 6	Data Word Size
0	7 Bit Communication
1	8 Bit Communication

Table 30 Parity Settings (without on-board LAN)

Switches		Parity
7	8	
0	0	No Parity
0	1	Odd Parity
1	1	Even Parity

One start bit and one stop bit are always used (not selectable).

Per default, the module will turn into 19200 baud, 8 data bit with no parity.

Special Settings

The special settings are required for specific actions (normally in a service case).

Boot-Resident

Firmware update procedures may require this mode in case of firmware loading errors (main firmware part).

If you use the following switch settings and power the instrument up again, the instrument firmware stays in the resident mode. It is not operable as a module. It only uses basic functions of the operating system for example, for communication. In this mode the main firmware can be loaded (using update utilities).

Table 31 Boot Resident Settings (without on-board LAN)

Mode Select	SW1	SW2	SW3	SW4	SW5	SW6	SW7	SW8
TEST/BOOT	1	1	0	0	1	0	0	0

Forced Cold Start

A forced cold start can be used to bring the module into a defined mode with default parameter settings.

CAUTION

Loss of data

Forced cold start erases all methods and data stored in the non-volatile memory. Exceptions are calibration settings, diagnosis and repair log books which will not be erased.

→ Save your methods and data before executing a forced cold start.

If you use the following switch settings and power the instrument up again, a forced cold start has been completed.

Table 32 Forced Cold Start Settings (without on-board LAN)

Mode Select	SW1	SW2	SW3	SW4	SW5	SW6	SW7	SW8
TEST/BOOT	1	1	0	0	0	0	0	1

Optional Interface Boards


BCD / External Contact Board

The Agilent 1200 Infinity Series modules have one optional board slot that allows to add an interface board to the modules. Some modules do not have this interface slot. Refer to “Interfaces” on page 183 for details.

Optional Interface Boards

p/n	Description
G1351-68701	Interface board (BCD) with external contacts and BCD outputs
2110-0004	Fuse for BCD board, 250 mA

The BCD board provides a BCD output for the bottle number of the Agilent 1200 Series autosampler and four external contacts. The external contact closure contacts are relay contacts. The maximum settings are: 30 V (AC/DC); 250 mA (fused).

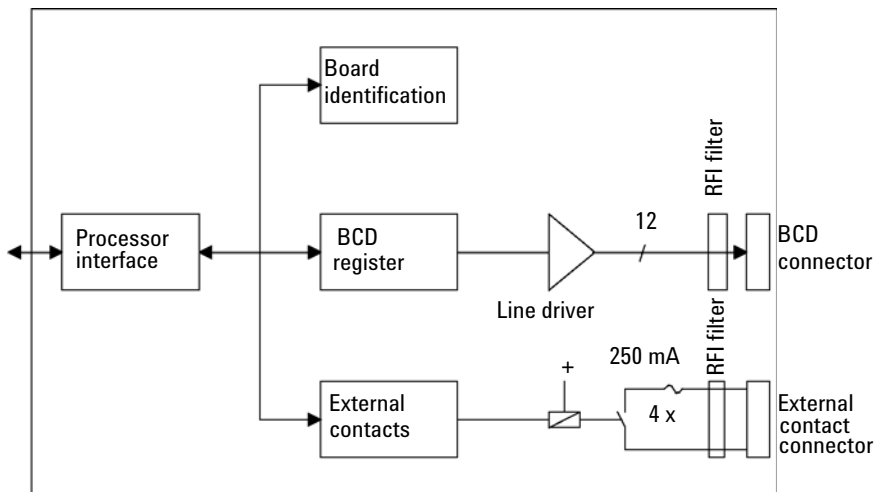

There are general purpose cables available to connect the BCD output, see “[BCD Cables](#)” on page 171 and the external outputs, see “[External Contact Cable](#)” on page 174 to external devices.

Table 33 Detailed connector layout (1200)

Pin	Signal name	BCD digit
1	BCD 5	20
2	BCD 7	80
3	BCD 6	40
4	BCD 4	10
5	BCD 0	1
6	BCD 3	8
7	BCD 2	4
8	BCD 1	2
9	Digital ground	
10	BCD 11	800
11	BCD 10	400
12	BCD 9	200
13	BCD 8	100
15	+5V	Low

LAN Communication Interface Board

The Agilent modules have one optional board slot that allows to add an interface board to the modules. Some modules do not have this interface slot. Refer to “[Interfaces](#)” on page 183 for details.

p/n	Description
G1369B or G1369-60002	Interface board (LAN)
OR G1369C or G1369-60012	Interface board (LAN)

NOTE

One board is required per Agilent 1260 Infinity instrument. It is recommended to add the LAN board to the detector with highest data rate.

NOTE

For the configuration of the G1369 LAN Communication Interface card refer to its documentation.

The following cards can be used with the Agilent 1260 Infinity modules.

Table 34 LAN Boards

Type	Vendor	Supported networks
Interface board (LAN) (G1369B or G1369-60002) or Interface board (LAN) (G1369C or G1369-60012)	Agilent Technologies	Fast Ethernet, Ethernet/802.3, RJ-45 (10/100Base-TX) <i>recommended for re-ordering</i>
LAN Communication Interface board (G1369A or G1369-60001)	Agilent Technologies	Fast Ethernet, Ethernet/802.3, RJ-45 (10/100Base-TX) <i>(obsolete)</i>
J4106A ¹	Hewlett Packard	Ethernet/802.3, RJ-45 (10Base-T)
J4105A ¹	Hewlett Packard	Token Ring/802.5, DB9, RJ-45 (10Base-T)
J4100A ¹	Hewlett Packard	Fast Ethernet, Ethernet/802.3, RJ-45 (10/100Base-TX) + BNC (10Base2)

¹ These cards may be no longer orderable. Minimum firmware of these Hewlett Packard JetDirect cards is A.05.05.

Recommended LAN Cables

p/n	Description
5023-0203	Cross-over network cable, shielded, 3 m (for point to point connection)
5023-0202	Twisted pair network cable, shielded, 7 m (for point to point connection)

Instrument Layout

The industrial design of the module incorporates several innovative features. It uses Agilent's E-PAC concept for the packaging of electronics and mechanical assemblies. This concept is based upon the use of expanded polypropylene (EPP) layers of foam plastic spacers in which the mechanical and electronic boards components of the module are placed. This pack is then housed in a metal inner cabinet which is enclosed by a plastic external cabinet. The advantages of this packaging technology are:

- virtual elimination of fixing screws, bolts or ties, reducing the number of components and increasing the speed of assembly/disassembly,
- the plastic layers have air channels molded into them so that cooling air can be guided exactly to the required locations,
- the plastic layers help cushion the electronic and mechanical parts from physical shock, and
- the metal inner cabinet shields the internal electronics from electromagnetic interference and also helps to reduce or eliminate radio frequency emissions from the instrument itself.

Early Maintenance Feedback

Maintenance requires the exchange of components which are subject to wear or stress. Ideally, the frequency at which components are exchanged should be based on the intensity of usage of the module and the analytical conditions, and not on a predefined time interval. The early maintenance feedback (**EMF**) feature monitors the usage of specific components in the instrument, and provides feedback when the user-selectable limits have been exceeded. The visual feedback in the user interface provides an indication that maintenance procedures should be scheduled.

EMF Counters

EMF counters increment with use and can be assigned a maximum limit which provides visual feedback in the user interface when the limit is exceeded. Some counters can be reset to zero after the required maintenance procedure.

Using the EMF Counters

The user-settable **EMF** limits for the **EMF Counters** enable the early maintenance feedback to be adapted to specific user requirements. The useful maintenance cycle is dependent on the requirements for use. Therefore, the definition of the maximum limits need to be determined based on the specific operating conditions of the instrument.

Setting the EMF Limits

The setting of the **EMF** limits must be optimized over one or two maintenance cycles. Initially the default **EMF** limits should be set. When instrument performance indicates maintenance is necessary, take note of the values displayed by the **EMF counters**. Enter these values (or values slightly less than the displayed values) as **EMF** limits, and then reset the **EMF counters** to zero. The next time the **EMF counters** exceed the new **EMF** limits, the **EMF** flag will be displayed, providing a reminder that maintenance needs to be scheduled.

11 Hardware Information

Early Maintenance Feedback



12 Appendix

General Safety Information	202
The Waste Electrical and Electronic Equipment Directive	205
Lithium Batteries Information	206
Radio Interference	207
Sound Emission	208
Use of Solvents	209
Agilent Technologies on Internet	210






This appendix provides general safety and environmental information.



General Safety Information

Safety Symbols

Table 35 Safety Symbols

Symbol	Description
	The apparatus is marked with this symbol when the user should refer to the instruction manual in order to protect risk of harm to the operator and to protect the apparatus against damage.
	Indicates dangerous voltages.
	Indicates a protected ground terminal.
	Indicates eye damage may result from directly viewing the light produced by the deuterium lamp used in this product.
	The apparatus is marked with this symbol when hot surfaces are available and the user should not touch it when heated up.

WARNING

A WARNING

alerts you to situations that could cause physical injury or death.

- Do not proceed beyond a warning until you have fully understood and met the indicated conditions.

CAUTION

A CAUTION

alerts you to situations that could cause loss of data, or damage of equipment.

- Do not proceed beyond a caution until you have fully understood and met the indicated conditions.

General Safety Information

The following general safety precautions must be observed during all phases of operation, service, and repair of this instrument. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.

WARNING

Ensure the proper usage of the equipment.

The protection provided by the equipment may be impaired.

→ The operator of this instrument is advised to use the equipment in a manner as specified in this manual.

Safety Standards

This is a Safety Class I instrument (provided with terminal for protective earthing) and has been manufactured and tested according to international safety standards.

Operation

Before applying power, comply with the installation section. Additionally the following must be observed.

Do not remove instrument covers when operating. Before the instrument is switched on, all protective earth terminals, extension cords, auto-transformers, and devices connected to it must be connected to a protective earth via a ground socket. Any interruption of the protective earth grounding will cause a potential shock hazard that could result in serious personal injury. Whenever it is likely that the protection has been impaired, the instrument must be made inoperative and be secured against any intended operation.

Make sure that only fuses with the required rated current and of the specified type (normal blow, time delay, and so on) are used for replacement. The use of repaired fuses and the short-circuiting of fuse holders must be avoided.

Some adjustments described in the manual, are made with power supplied to the instrument, and protective covers removed. Energy available at many points may, if contacted, result in personal injury.

Any adjustment, maintenance, and repair of the opened instrument under voltage should be avoided whenever possible. When inevitable, this has to be carried out by a skilled person who is aware of the hazard involved. Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present. Do not replace components with power cable connected.

Do not operate the instrument in the presence of flammable gases or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.

Do not install substitute parts or make any unauthorized modification to the instrument.

Capacitors inside the instrument may still be charged, even though the instrument has been disconnected from its source of supply. Dangerous voltages, capable of causing serious personal injury, are present in this instrument. Use extreme caution when handling, testing and adjusting.

When working with solvents, observe appropriate safety procedures (for example, goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet by the solvent vendor, especially when toxic or hazardous solvents are used.

The Waste Electrical and Electronic Equipment Directive

Abstract

The Waste Electrical and Electronic Equipment (WEEE) Directive (2002/96/EC), adopted by EU Commission on 13 February 2003, is introducing producer responsibility on all electric and electronic appliances starting with 13 August 2005.

NOTE

This product complies with the WEEE Directive (2002/96/EC) marking requirements. The affixed label indicates that you must not discard this electrical/electronic product in domestic household waste.

Product Category:

With reference to the equipment types in the WEEE Directive Annex I, this product is classed as a Monitoring and Control Instrumentation product.



NOTE

Do not dispose off in domestic household waste

To return unwanted products, contact your local Agilent office, or see www.agilent.com for more information.

Lithium Batteries Information

WARNING

Lithium batteries may not be disposed-off into the domestic waste. Transportation of discharged Lithium batteries through carriers regulated by IATA/ICAO, ADR, RID, IMDG is not allowed.

Danger of explosion if battery is incorrectly replaced.

- Discharged Lithium batteries shall be disposed off locally according to national waste disposal regulations for batteries.
 - Replace only with the same or equivalent type recommended by the equipment manufacturer.
-



WARNING

Lithiumbatteri - Eksplosionsfare ved fejlagtig håndtering.

Udskiftning må kun ske med batteri af samme fabrikat og type.

- Lever det brugte batteri tilbage til leverandøren.
-

WARNING

Lithiumbatteri - Eksplosionsfare.

Ved udskiftning benyttes kun batteri som anbefalt av apparatfabrikanten.

- Brukt batteri returneres apparatleverandøren.
-

NOTE

Bij dit apparaat zijn batterijen geleverd. Wanneer deze leeg zijn, moet u ze niet weggooien maar inleveren als KCA.

Radio Interference

Cables supplied by Agilent Technologies are screened to provide optimized protection against radio interference. All cables are in compliance with safety or EMC regulations.

Test and Measurement

If test and measurement equipment is operated with unscreened cables, or used for measurements on open set-ups, the user has to assure that under operating conditions the radio interference limits are still met within the premises.

Sound Emission

Manufacturer's Declaration

This statement is provided to comply with the requirements of the German Sound Emission Directive of 18 January 1991.


This product has a sound pressure emission (at the operator position) < 70 dB.

- Sound Pressure $L_p < 70$ dB (A)
- At Operator Position
- Normal Operation
- According to ISO 7779:1988/EN 27779/1991 (Type Test)

Use of Solvents

Observe the following recommendations on the use of solvents.

- Brown glass ware can avoid growth of algae.
- Avoid the use of the following steel-corrosive solvents:
 - Solutions of alkali halides and their respective acids (for example, lithium iodide, potassium chloride, and so on),
 - High concentrations of inorganic acids like sulfuric acid and nitric acid, especially at higher temperatures (if your chromatography method allows, replace by phosphoric acid or phosphate buffer which are less corrosive against stainless steel),
 - Halogenated solvents or mixtures which form radicals and/or acids, for example:



This reaction, in which stainless steel probably acts as a catalyst, occurs quickly with dried chloroform if the drying process removes the stabilizing alcohol,

- Chromatographic grade ethers, which can contain peroxides (for example, THF, dioxane, di-isopropyl ether) such ethers should be filtered through dry aluminium oxide which adsorbs the peroxides,
- Solvents containing strong complexing agents (e.g. EDTA),
- Mixtures of carbon tetrachloride with 2-propanol or THF.

Agilent Technologies on Internet

For the latest information on products and services visit our worldwide web site on the Internet at:

<http://www.agilent.com>

Index

8

8-bit configuration switch
without On-Board LAN 190

A

advanced operating modes 22
Agilent Lab Advisor software 105
Agilent Lab Advisor 105
Agilent
on internet 210
algae 209
ambient non-operating temperature 31
ambient operating temperature 31
analog signal 187
analog
cable 166
apg remote 188

B

battery
safety information 206
BCD board
external contacts 194
BCD
cable 171
bench space 30
board
HP JetDirect card 196
boards
LAN card 196
bypass 14

C

cable
analog 166
BCD 171
CAN 173
connecting APG remote 40
connecting CAN 40
connecting LAN 40
connecting the ChemStation 40
connecting the power 40
external contact 174
LAN 173
remote 168
RS-232 175
cables
analog 164
BCD 164
CAN 165
external contact 165
LAN 165
overview 164
remote 164
RS-232 165
CAN
cable 173
capillaries 52
choice of vials and caps 80
cleaning 133
Communication settings
RS-232C 191
compensation sensor open 113
compensation sensor short 114
condensation 30
configuration
one stack 37, 37

two stack 39

D

damaged packaging 34
delivery checklist 34, 34
dimensions 31
draw speed 80, 80
draw 80, 92

E

eject speed 80, 80
EJECT 80
electrical connections
descriptions of 181
electronic waste 205
EMF
early maintenance feedback 199
error messages
arm movement 117
compensation sensor open 113
compensation sensor short 114
fan failed 114
front door error 116
ignition without cover 115, 115
initialization failed 122
invalid vial position 125
leak sensor open 113
leak sensor short 112
leak 115
lost CAN partner 112
metering home failed 123
missing vial 121
motor temperature 124
needle lock failed 119
needle to needle seat position 120

Index

- peristaltic pump error 126
- remote timeout 111
- shutdown 111
- timeout 110
- valve to bypass failed 118
- valve to mainpass failed 118
- vessel error 126
- vessel stuck to needle 127
- external contact
 - cable 174
- external contacts
 - BCD board 194
- F**
- failure 86
- fan failed 114
- firmware
 - description 178
 - main system 178
 - resident system 178
 - update tool 179
 - updates 179, 154, 154
 - upgrade/downgrade 154
 - upgrade/downgrade 154
- flow connections 52
- frequency range 31
- G**
- general error messages 110
- H**
- HP JetDirect card 196
- humidity 31
- I**
- injection sequence 14
- injection valve 10, 16, 18
- injection volume precision 80
- injection volume 80
- injection volumes less than 2 μ l 80
- injection volumes 80
- installation
 - bench space 30
- installing the autosampler
 - flow connections 52
 - interface cables 45
 - power cable 45
 - safety 45
 - sample trays 59
- installing the sample tray 54
- installing the thermostatted autosampler
 - interface cables 48
 - power cable 48
 - preparation 49
 - safety 48, 45
 - tray cover and front cover 56
- instrument layout 198
- interfaces 183
- internet 210
- introduction to the autosampler 10
- L**
- LAN
 - cable 173
 - communication interface board 196
- leak sensor open 113
- leak sensor short 112
- leak 115
- line frequency 31
- line voltage 31
- lithium batteries 206
- lost CAN partner 112
- low volume injections 80
- M**
- mainpass 14
- maintenance functions 86, 90, 134
 - step commands 92
- maintenance procedures 135
- maintenance
 - feedback 199
 - replacing firmware 154, 154
- manual control 92
- message
 - ignition without cover 115, 115
 - remote timeout 111
- metering device 16, 80
- missing parts 34
- move to location 92
- multi-draw option 10
- N**
- needle drive 16
- needle flush station 19
- needle into sample 92
- needle into seat 92
- needle lock 19
- needle up/mainpass 92
- needle up 92, 92
- needle/sample transport assembly 20
- non-operating altitude 31
- non-operating temperature 31
- numbering of vials 59
- O**
- operating Altitude 31
- operating modes 22
- operating temperature 31
- optimization
 - stack configuration 36
- optimizing performance
 - automated needle wash 80
 - delay volume 80
 - delay-volume adjustment 80
 - early maintenance 80
 - inject-valve seal 80
 - low-volume capillary kit 80

P

- park transport assembly 56
- parts and materials 34
 - transport assembly 156
 - vial trays and tray base 158
- parts identification
 - cables 163
- Peek seal 82
- performance specifications 32
- physical specifications 31
- plunger home 92
- power consideration 28
- power consumption 31
- power cords 29
- power supply indicator 88

R

- radio interference 207
- remote
 - cable 168
- repairs
 - maintenance procedures 135
 - metering plunger 146
 - metering seal 146
 - needle assembly 136
 - replacing firmware 154, 154
 - rotor seal 145
- rotor seal 82
- RS-232C
 - cable 175
 - communication settings 191

S

- safety class I 203
- safety information
 - lithium batteries 206
- safety
 - general information 203

- standards 31
- symbols 202
- sample trays 59
 - numbering of vial positions 60
- sampling sequence 12
- sampling unit 16
- seals 82
- shipping containers 34
- shipping 56
- shutdown 111
- site requirements
 - power cords 29
- solvents 209
- sound emission 208
- special interfaces 189
- special settings
 - boot-resident 193
 - forced cold start 193
- specification
 - physical 31
- specifications 32
- stack configuration
 - front view 39
 - rear view 40
- stator 18
- status indicators 88
- status indicator 86, 89
- step commands 92
- step functions 87
- system setup and installation
 - optimizing stack configuration 36

T

- Tefzel seal 82
- temperature sensor 115
- temperature 32
- thermostat 161
- theta-axis 20
- timeout 110

- transport assembly 20
- transport mechanism 10
- transporting the autosampler 56
- transport 56
- tray combinations 60
- trays 59
- troubleshooting
 - error messages 109

U

- unpacking the autosampler 34

V

- valve bypass 92
- valve capillaries 52
- valve mainpass 92
- Vespel seal 82
- vial contents temperature 32
- vial numbering 59
- vial racks 10
- vial tray 56
- vials 10
- viscous samples 80, 80
- voltage range 31

W

- waste
 - electrical and electronic equipment 205
- WEEE directive 205
- weight 31

X

- X-axis 20

Z

- Z-axis 20

In This Book

This manual contains user information about the Agilent 1260 Infinity High Performance Micro Autosampler. The manual describes the following:

- introduction to the sampler,
- site requirements and specifications,
- installing, configuring and using the autosampler,
- optimizing performance,
- troubleshooting and diagnostics,
- error information,
- maintenance,
- parts and materials,
- information on cables,
- safety and legal information.

© Agilent Technologies 2006, 2008, 2010, 2013

Printed in Germany
11/2013



G1377-90001



Agilent Technologies